

METHOD AND SYSTEM FOR CONTROL OF A PATIENT'S BODY
TEMPERATURE . . . HEAT EXCHANGE CATHETER

Machold et al. Div. of 09/707,257

Docket No. RADME-65146

1 / 36

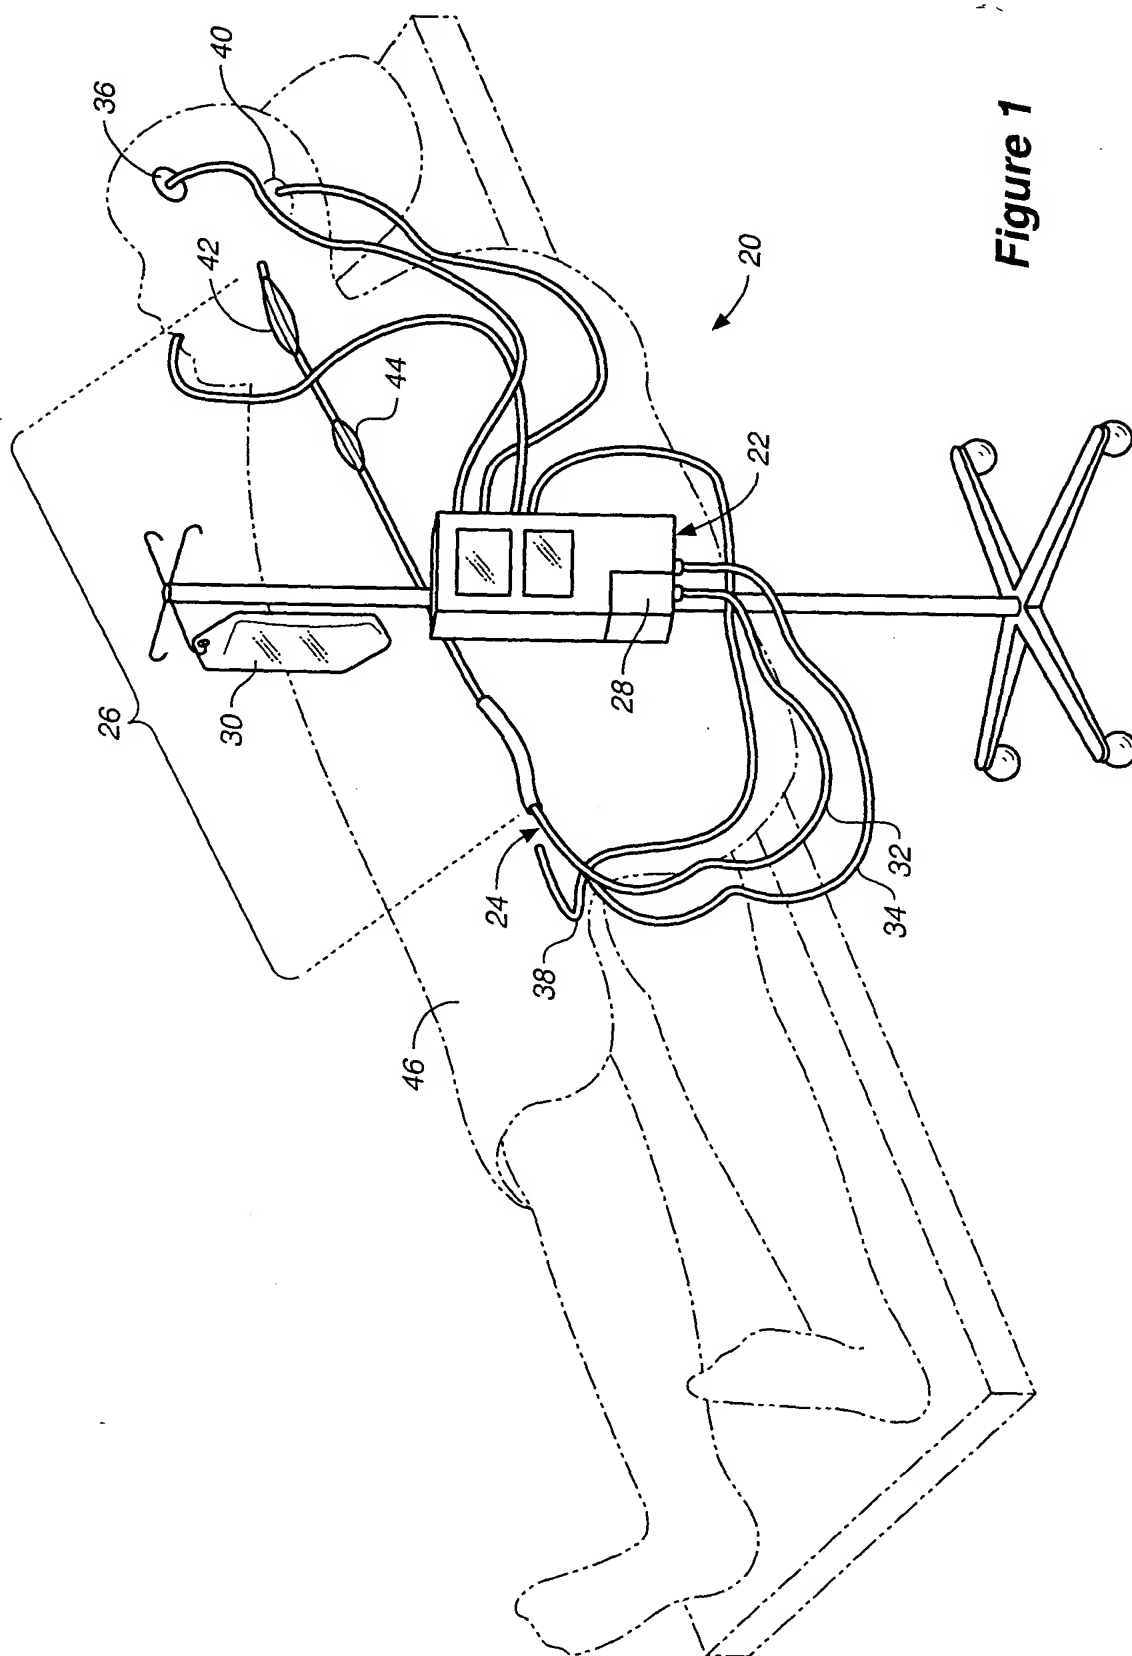


Figure 1

2 / 36

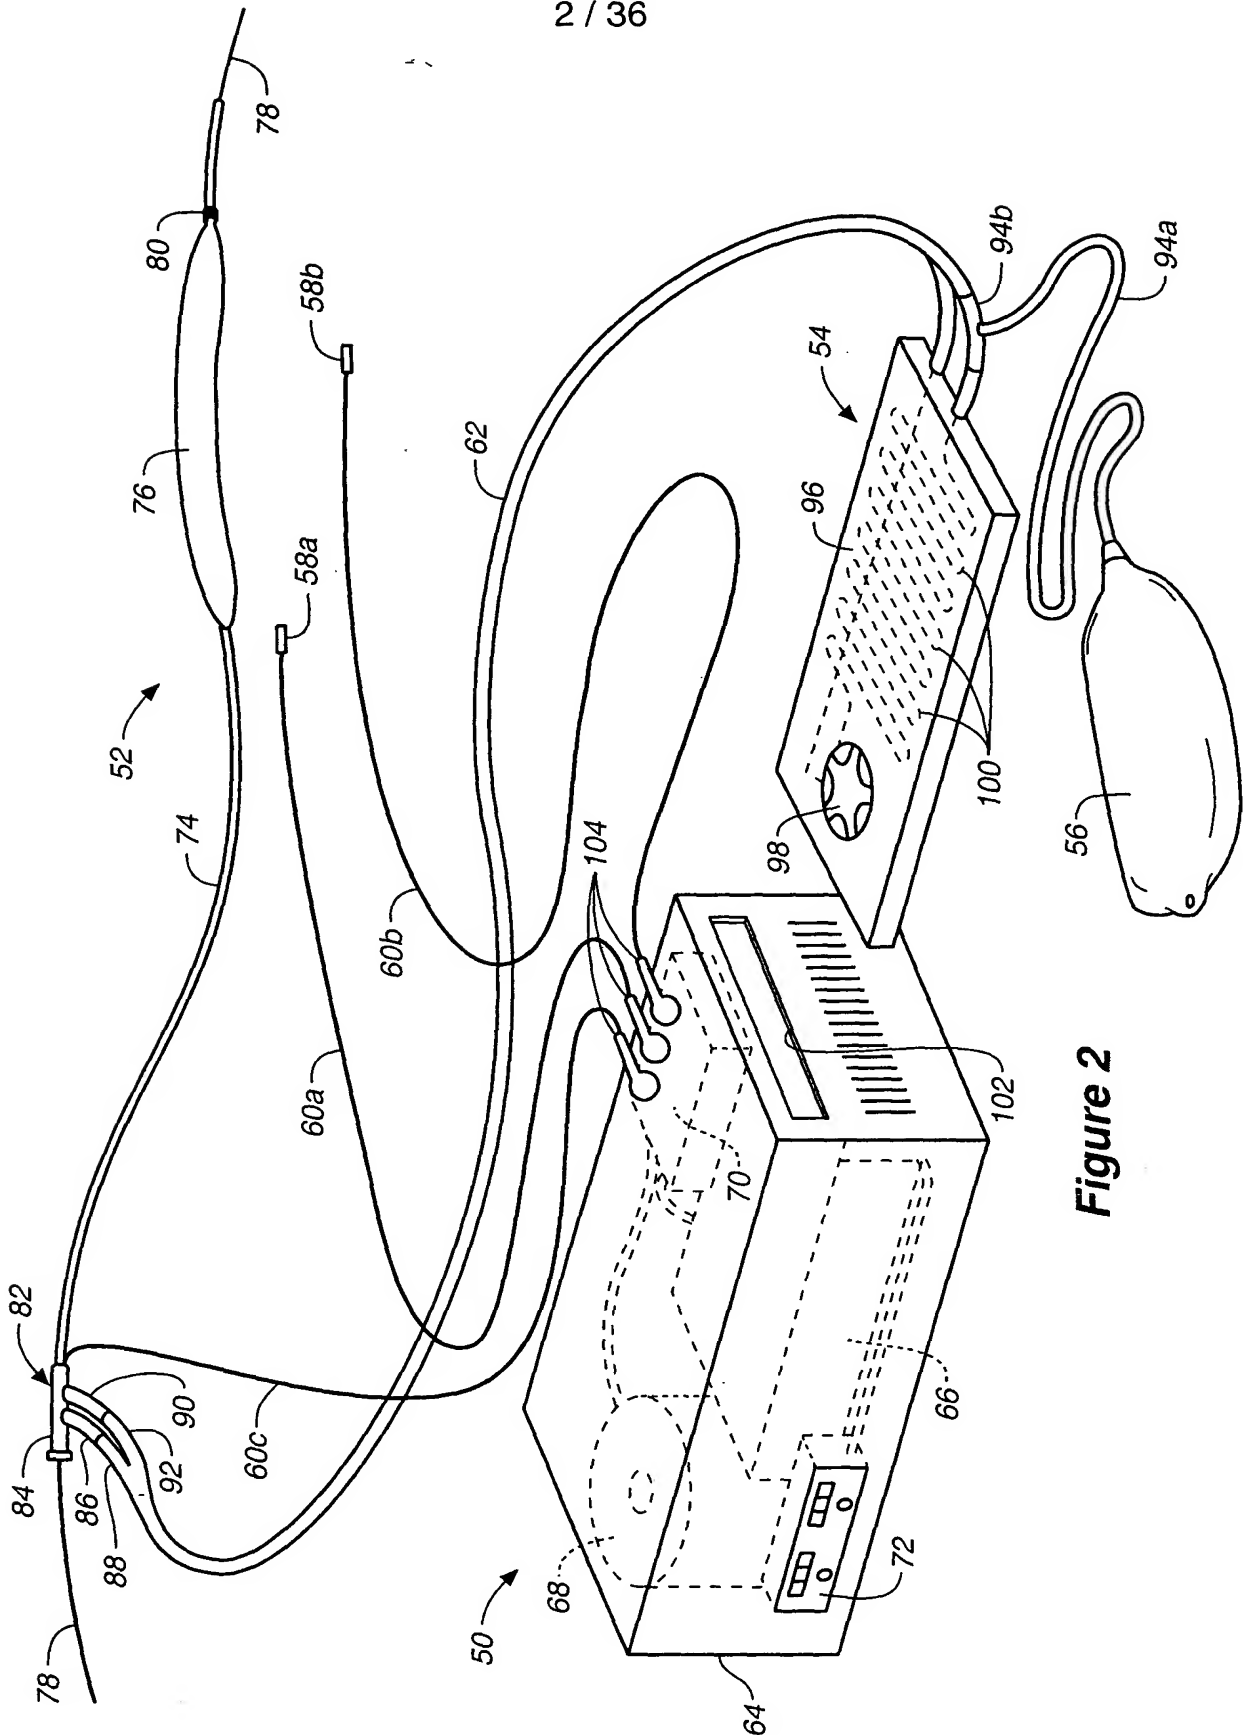


Figure 2

3 / 36

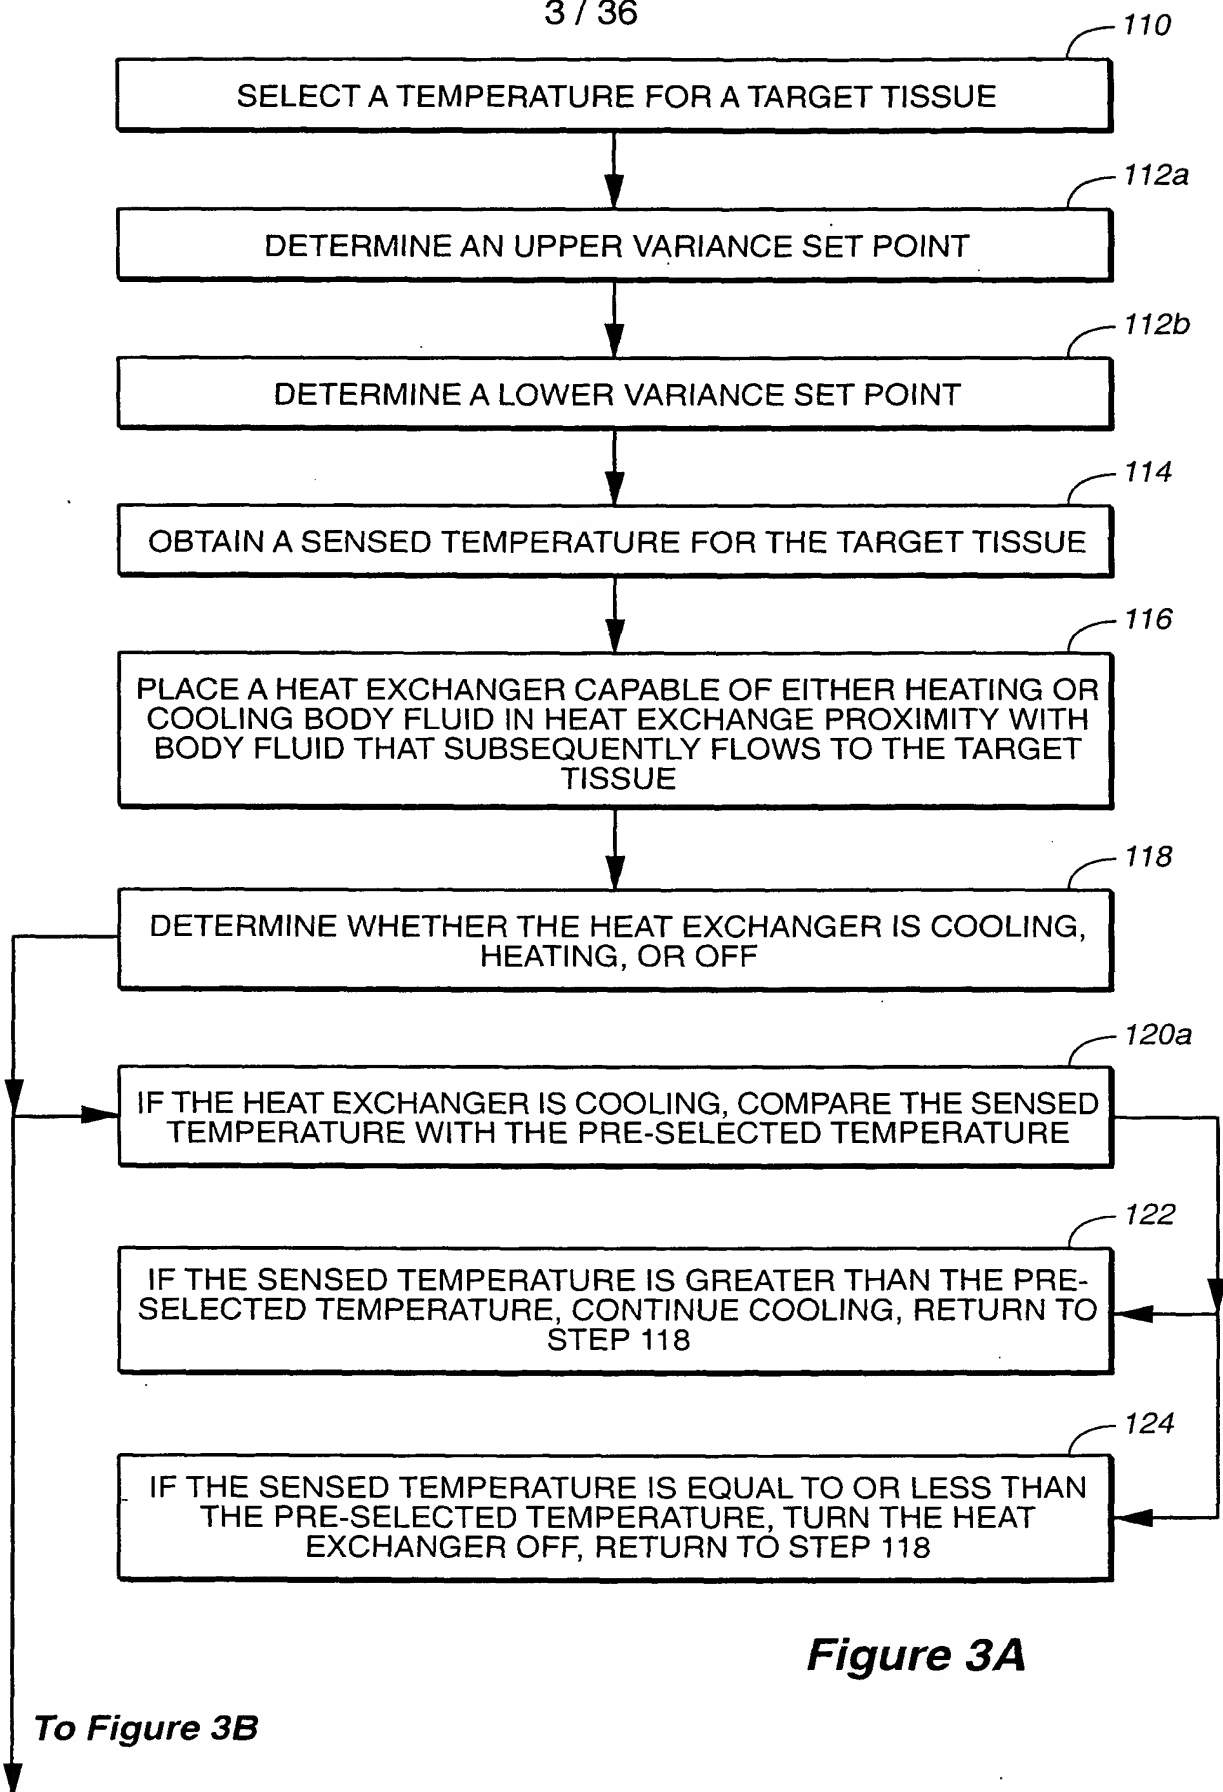


Figure 3A

From Figure 3A

4 / 36


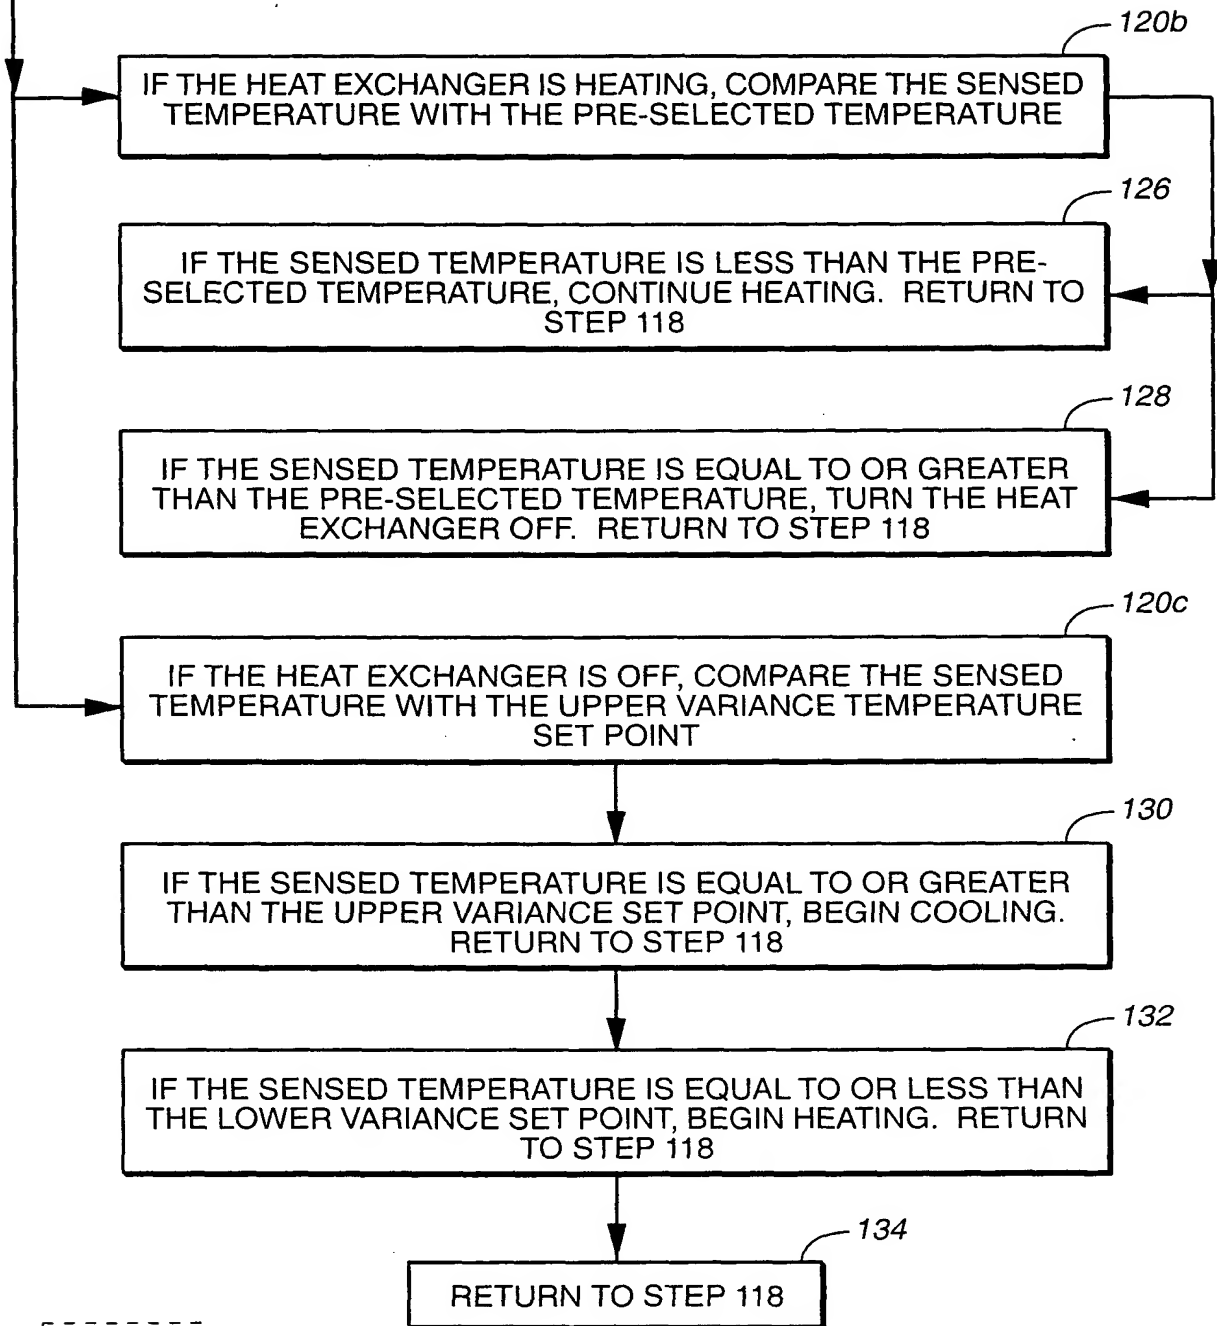


Figure 3B

FIG. 3A

FIG. 3B

FIG. 3

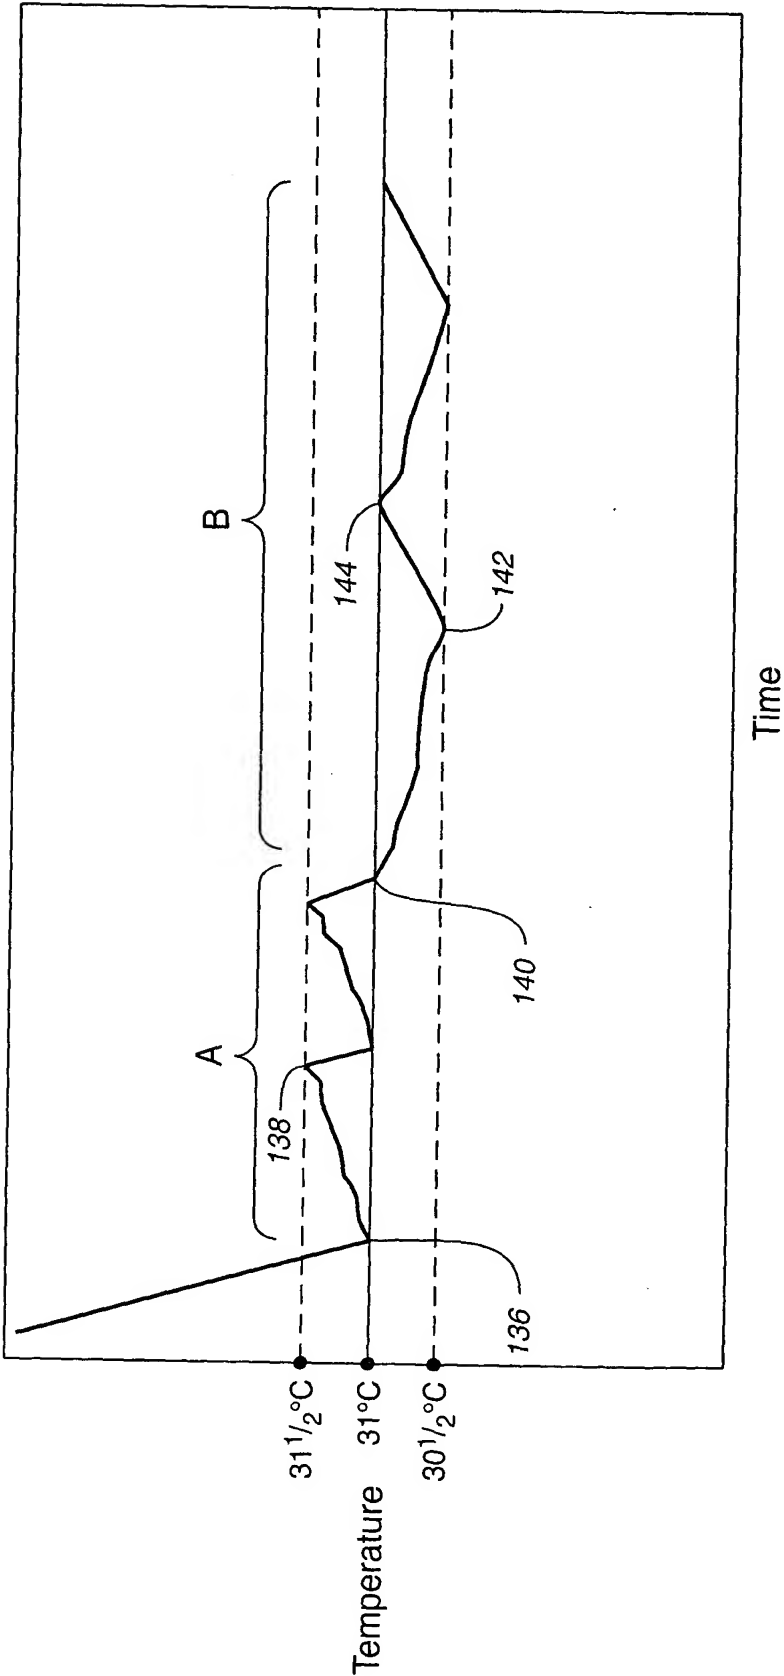

31 °C = Pre-selected temperature
31 1/2 °C = Upper variance set point
30 1/2 °C = Lower variance set point

Figure 4

6 / 36

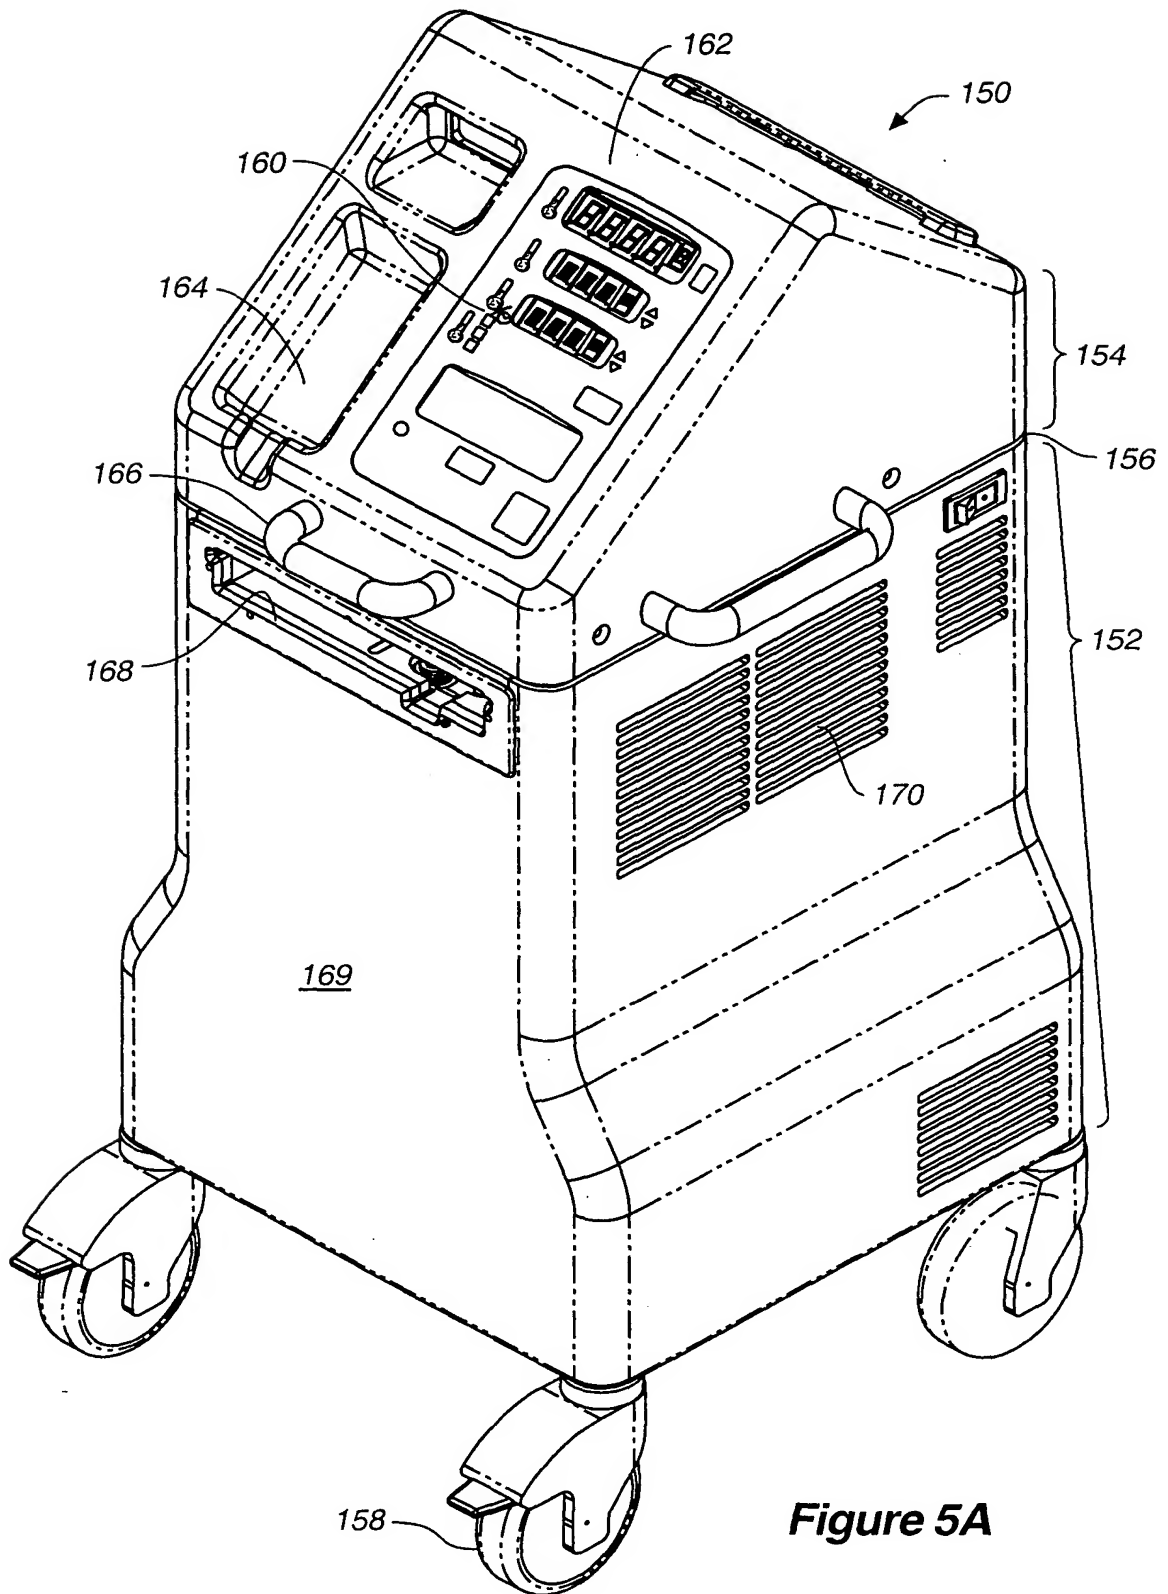


Figure 5A

+

7 / 36

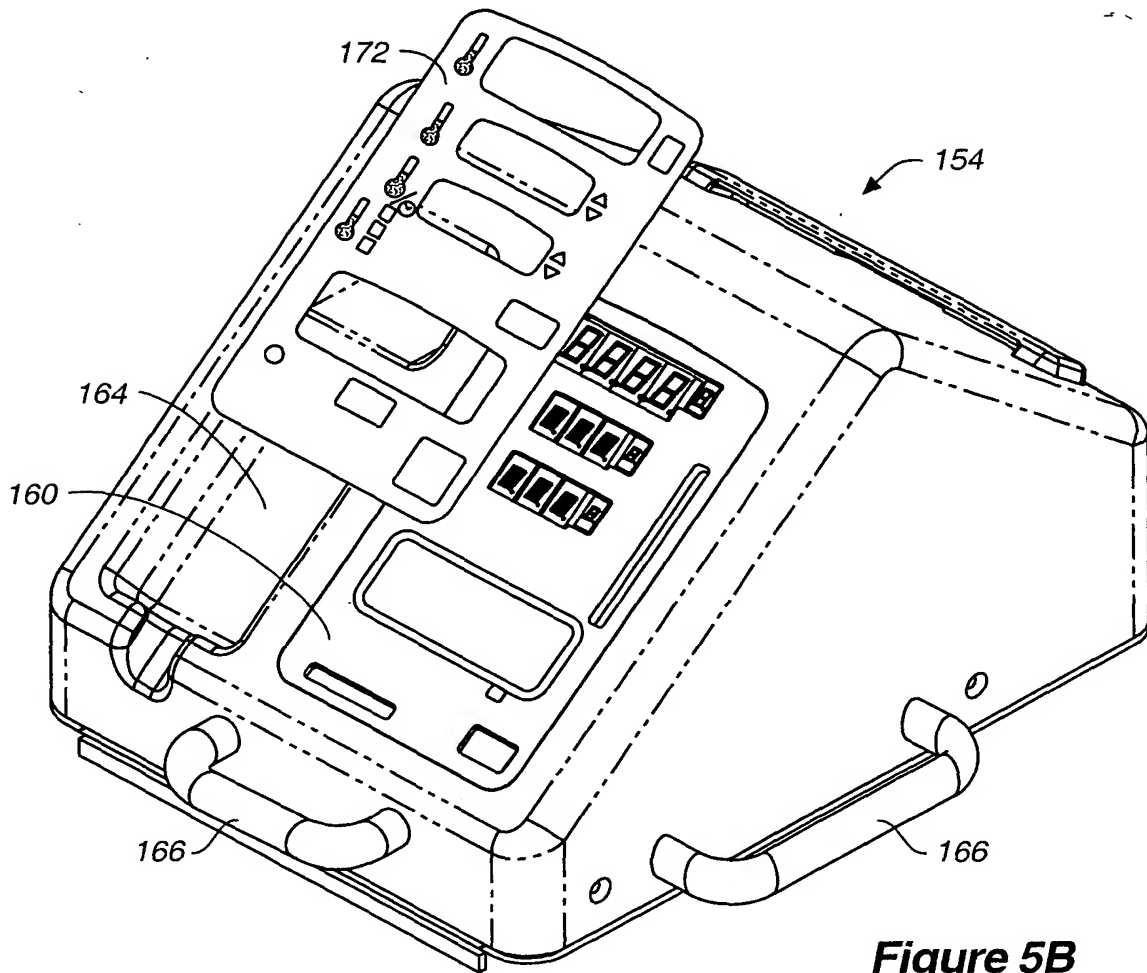


Figure 5B

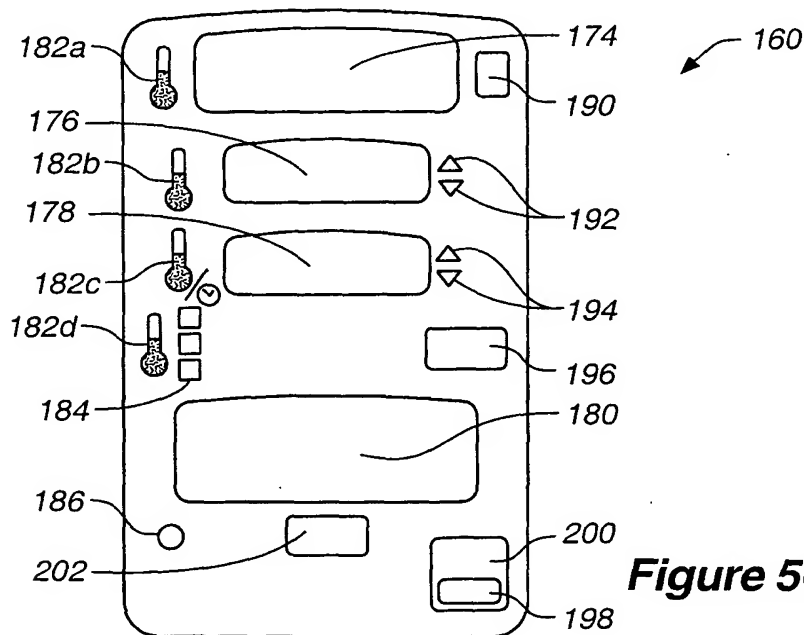


Figure 5C

+

8 / 36

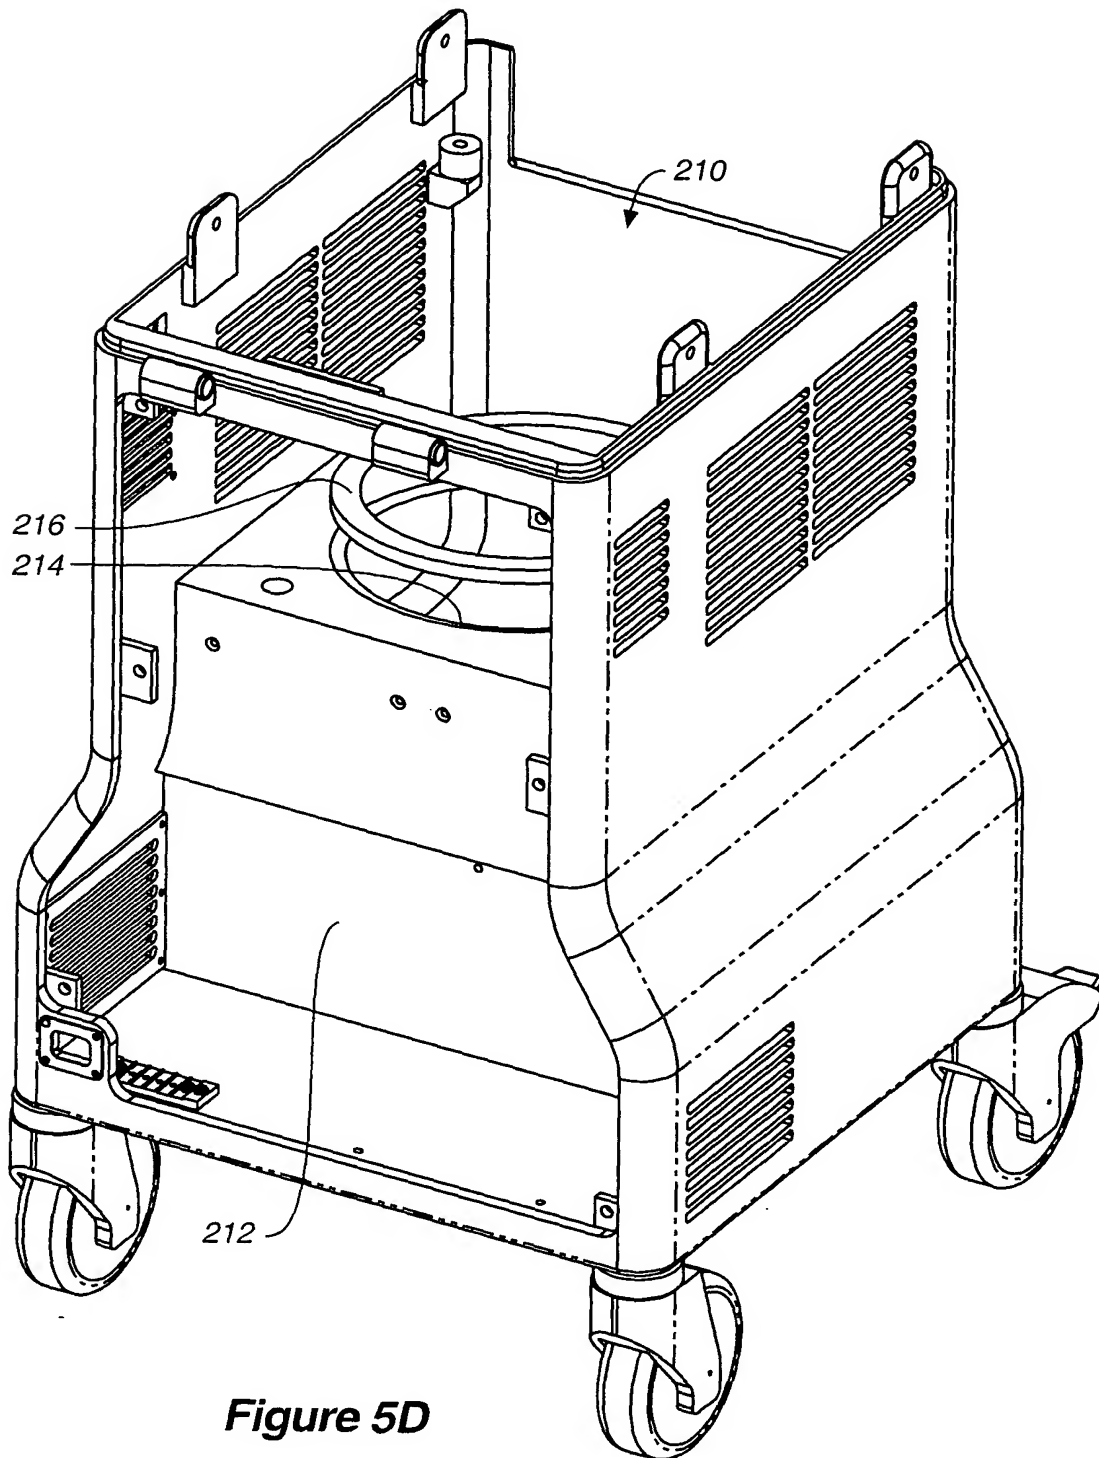


Figure 5D

9 / 36

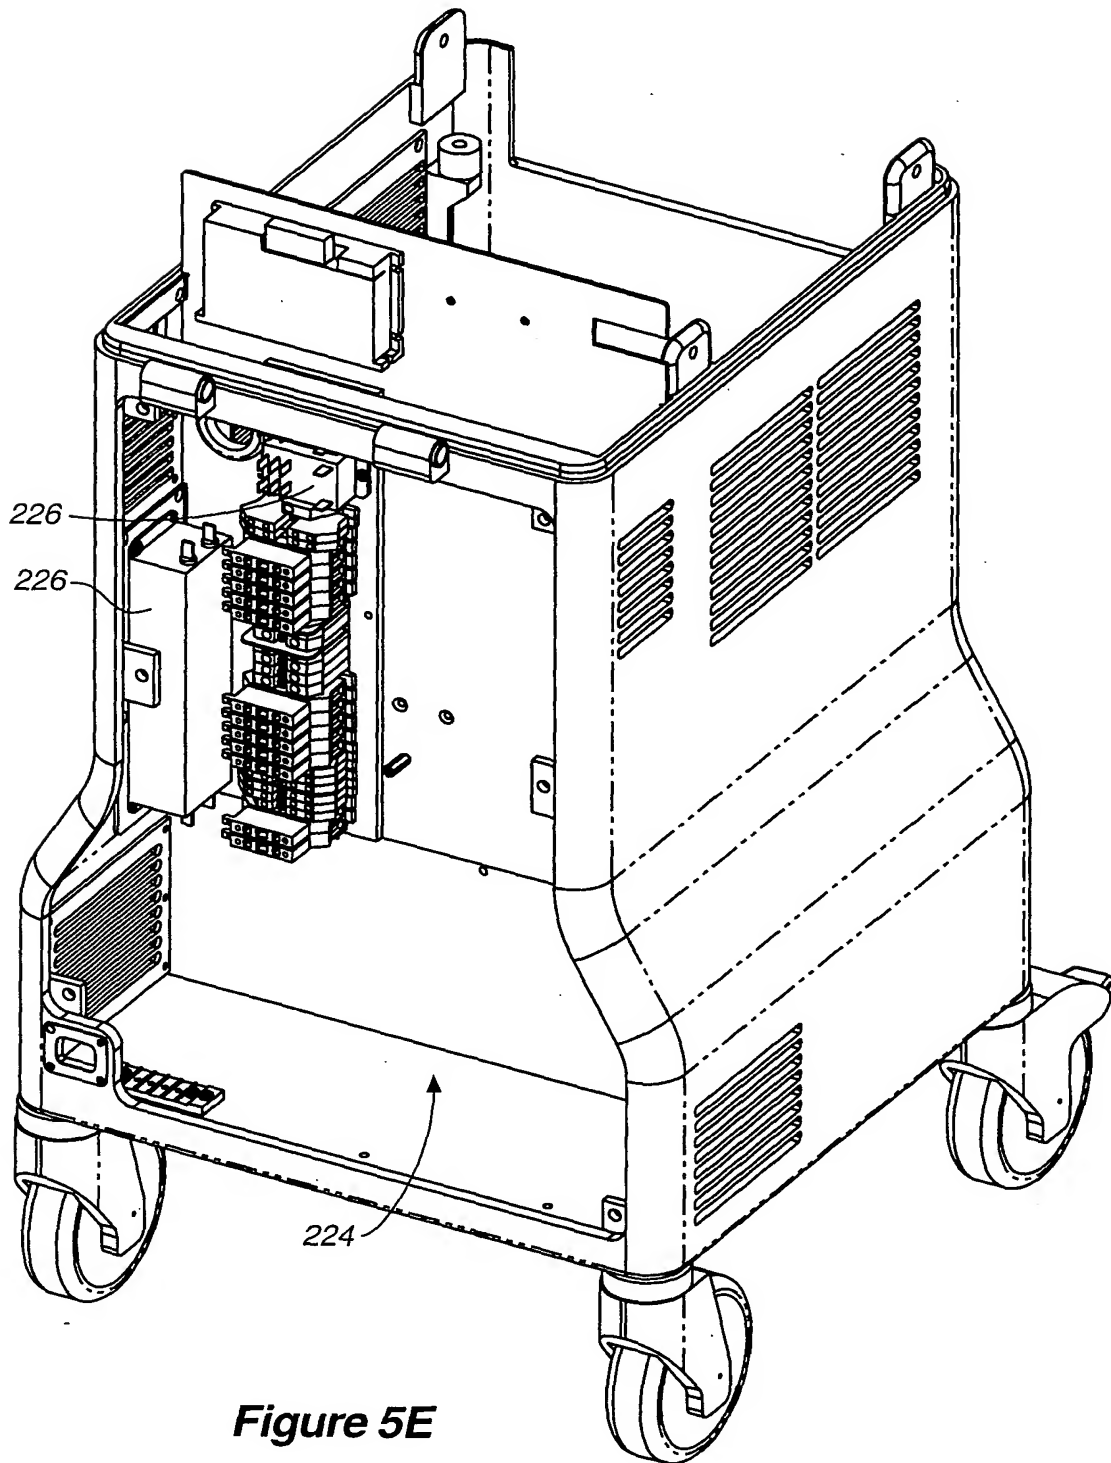


Figure 5E

10 / 36


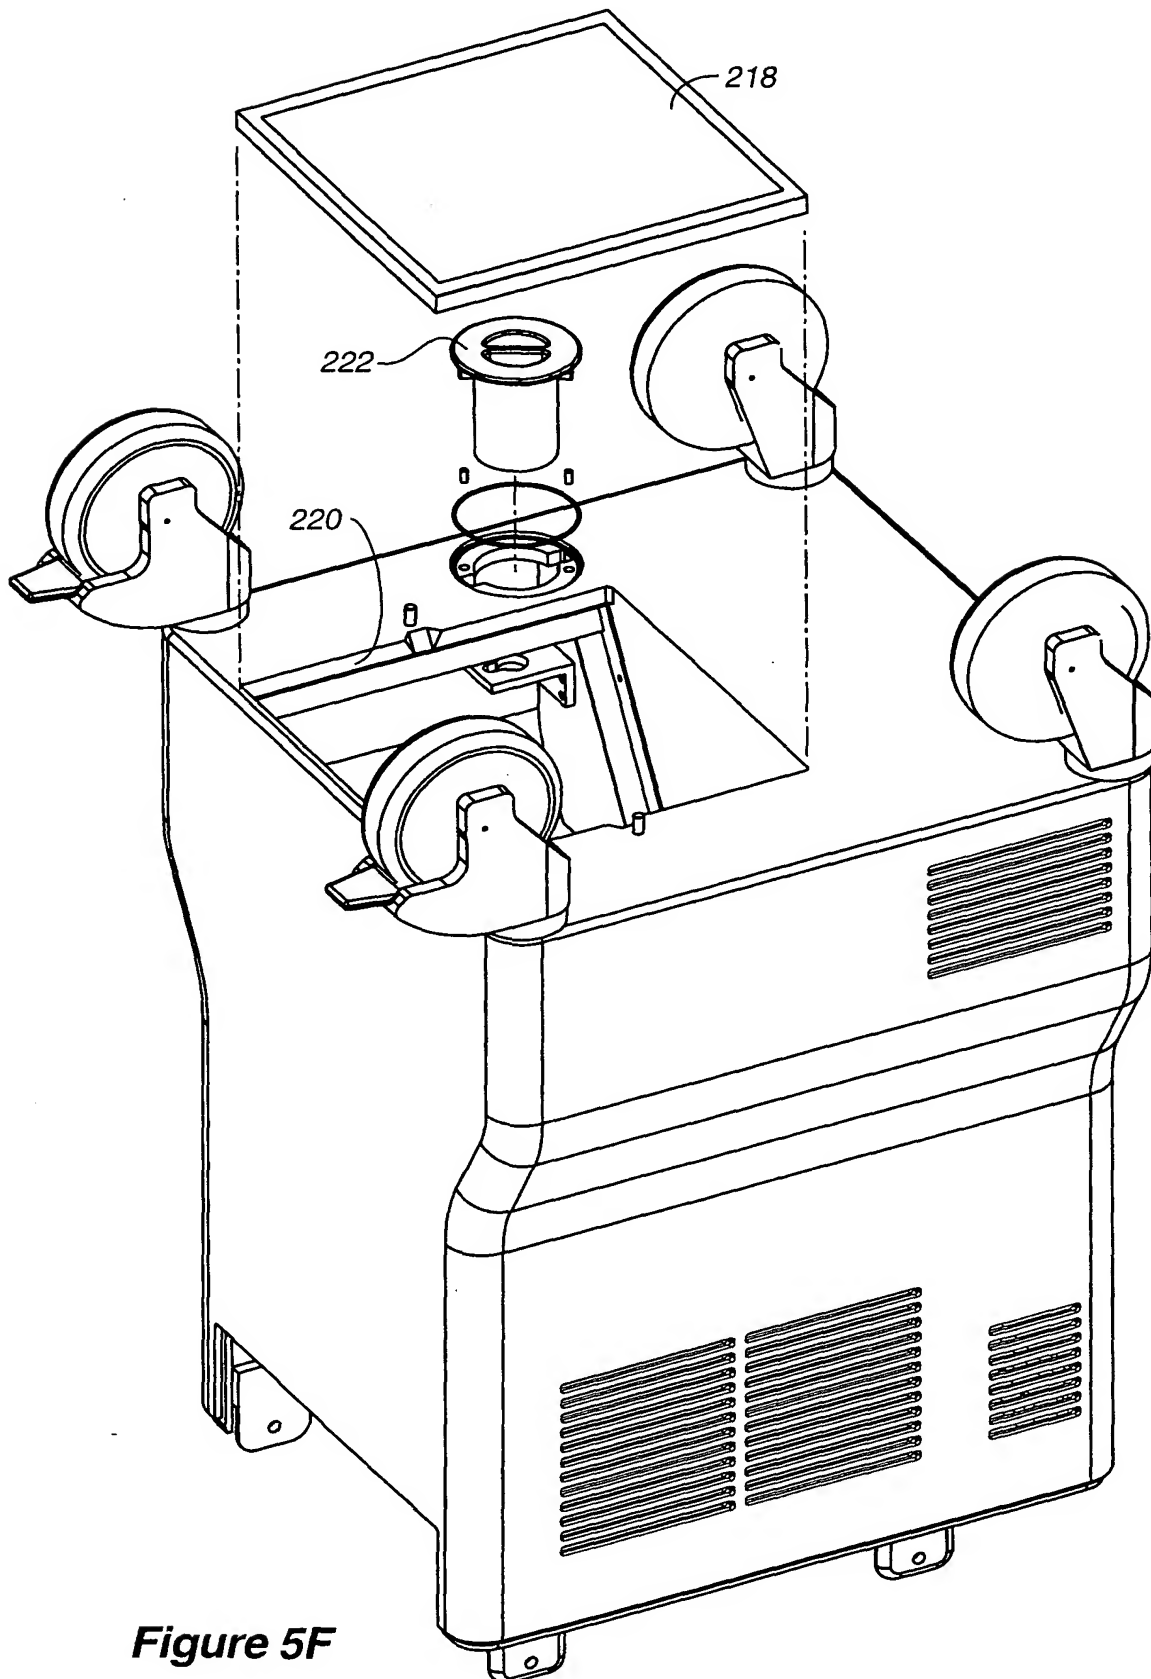


Figure 5F

11 / 36

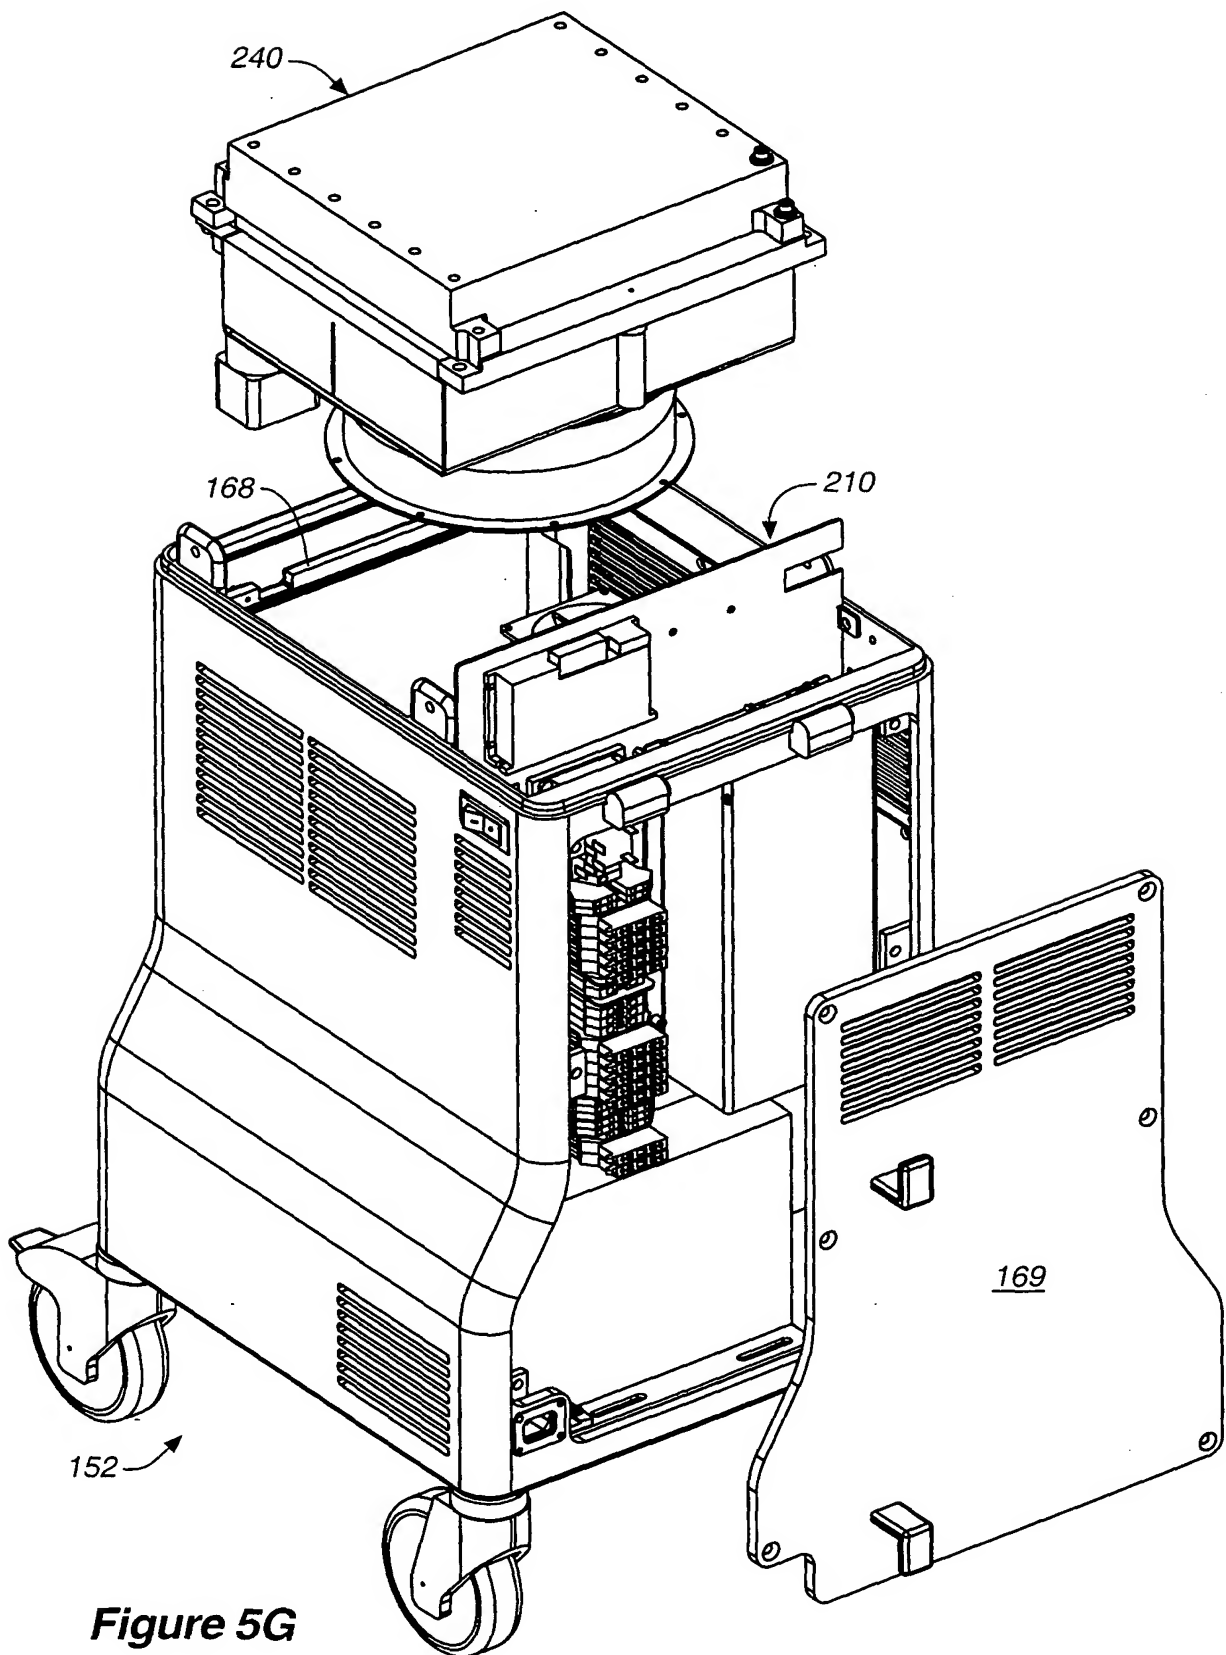

12 / 36

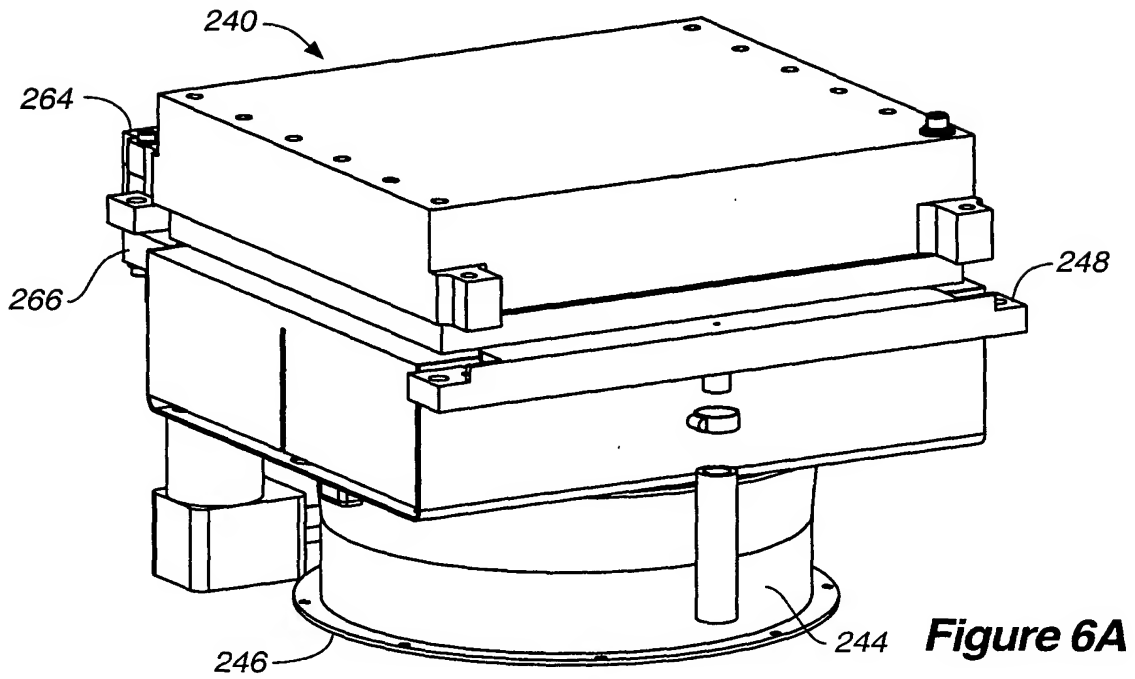


Figure 6A

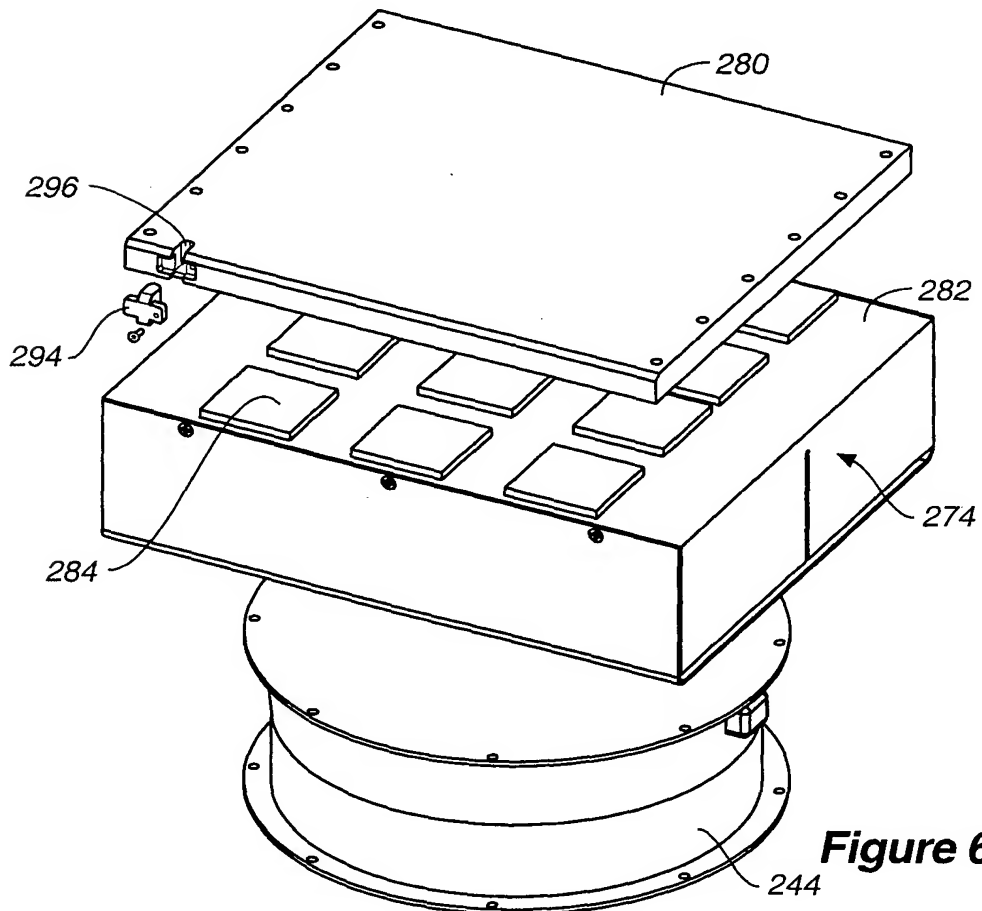


Figure 6C

13 / 36

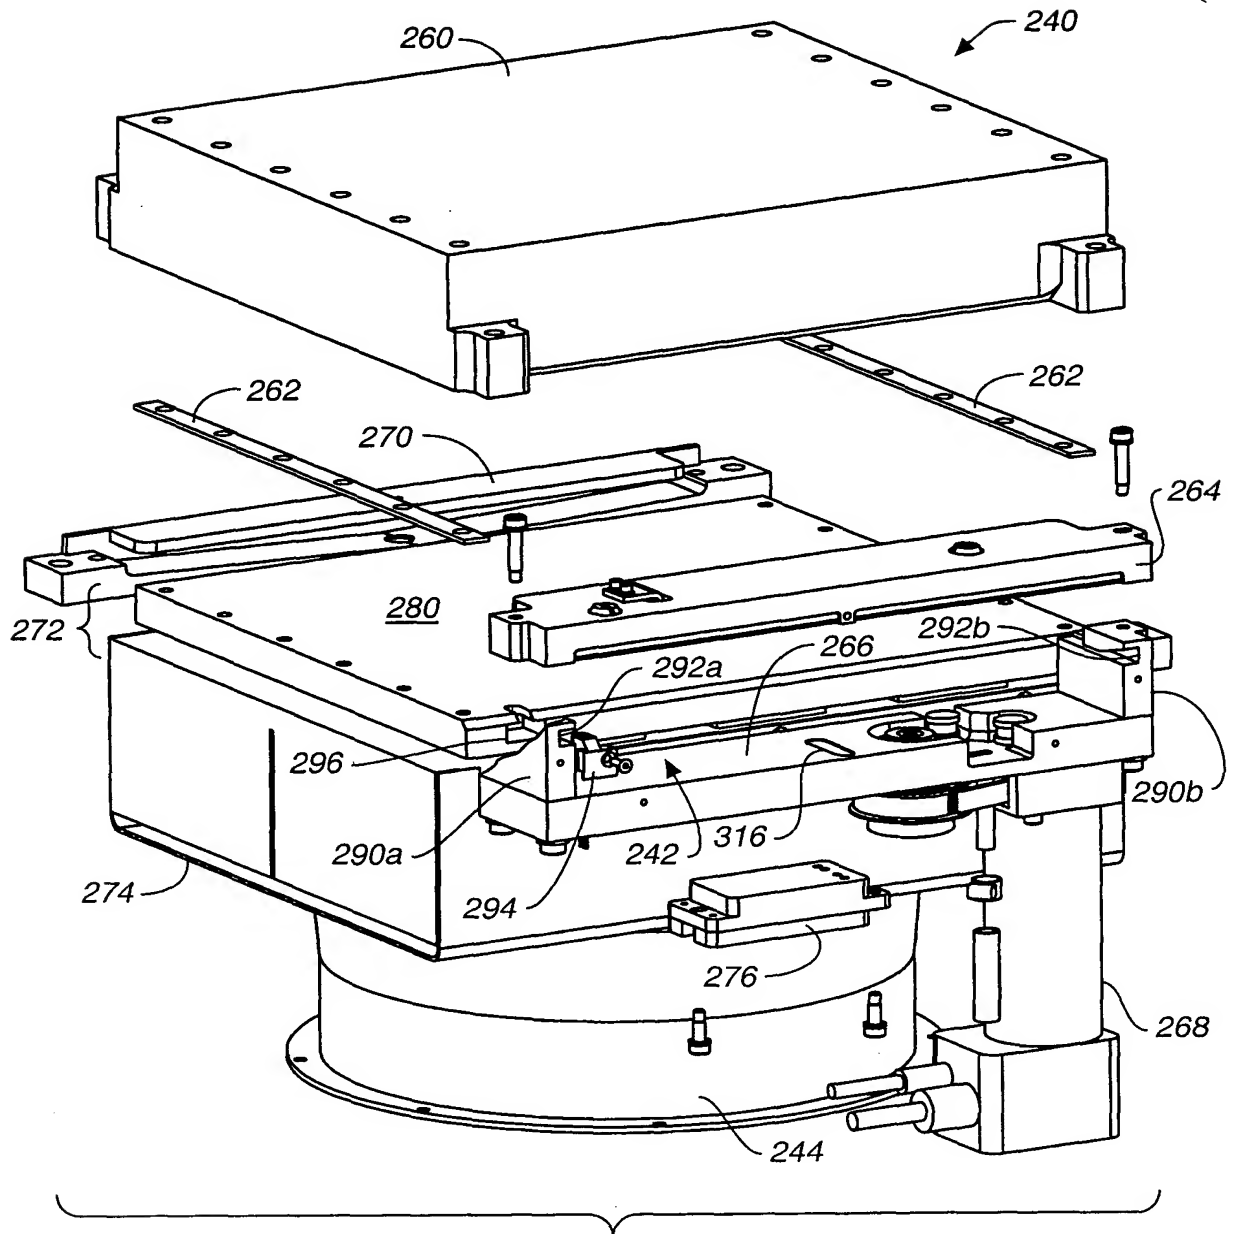


Figure 6B

14 / 36

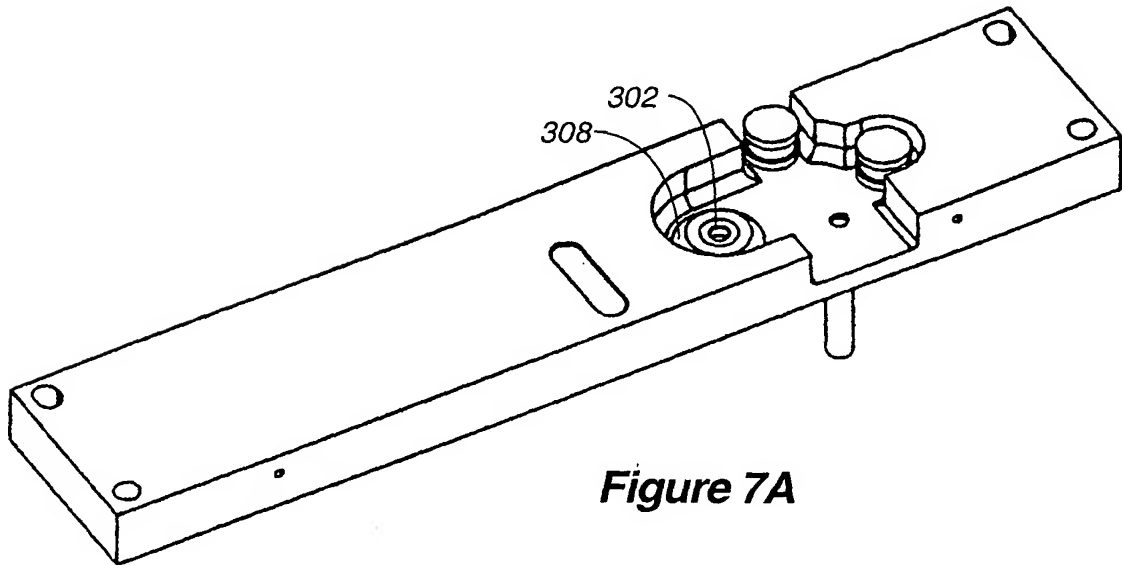


Figure 7A

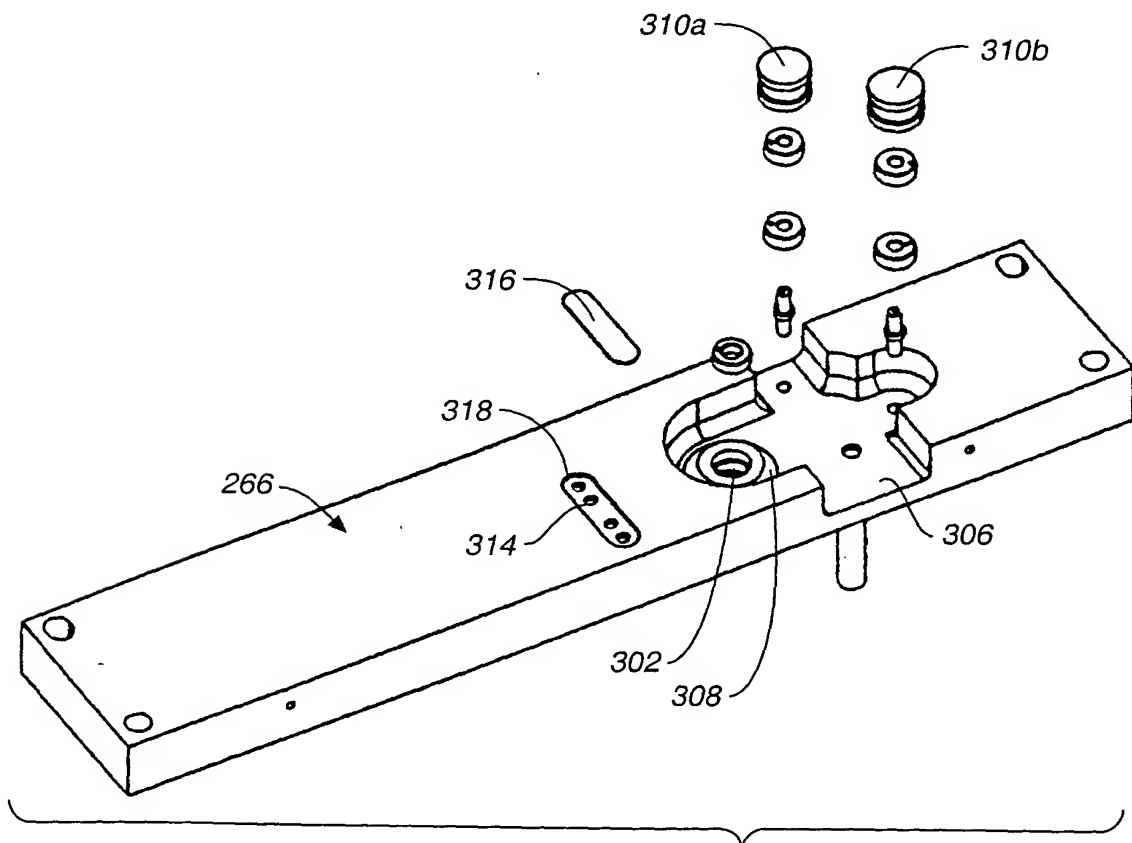


Figure 7B

15 / 36

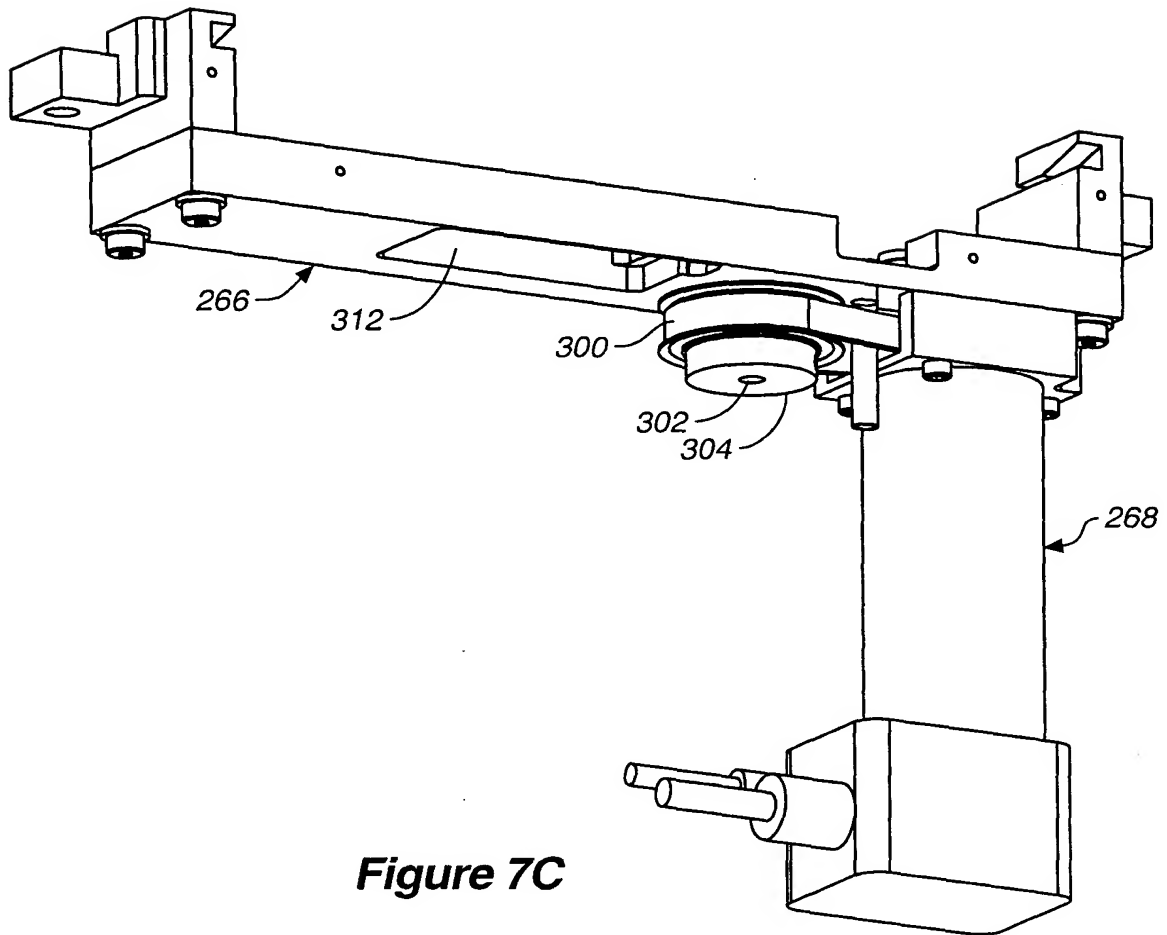


Figure 7C

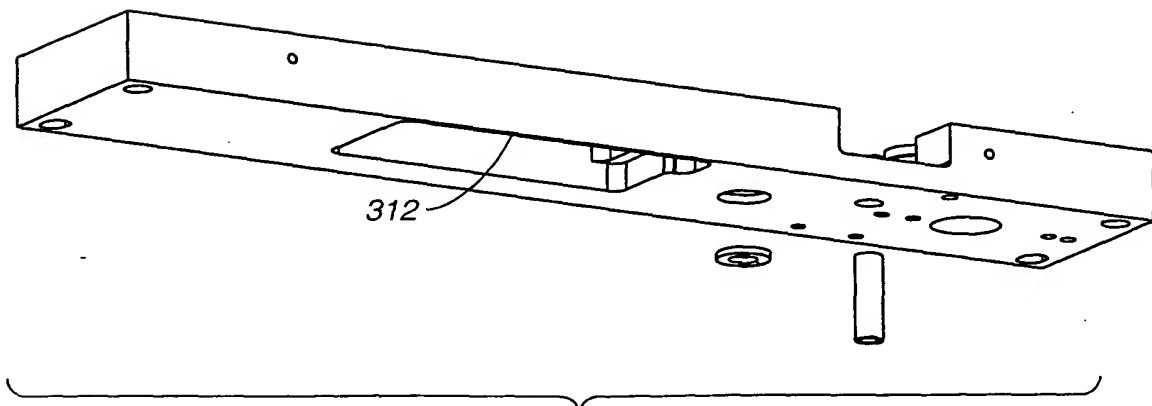


Figure 7D

16 / 36

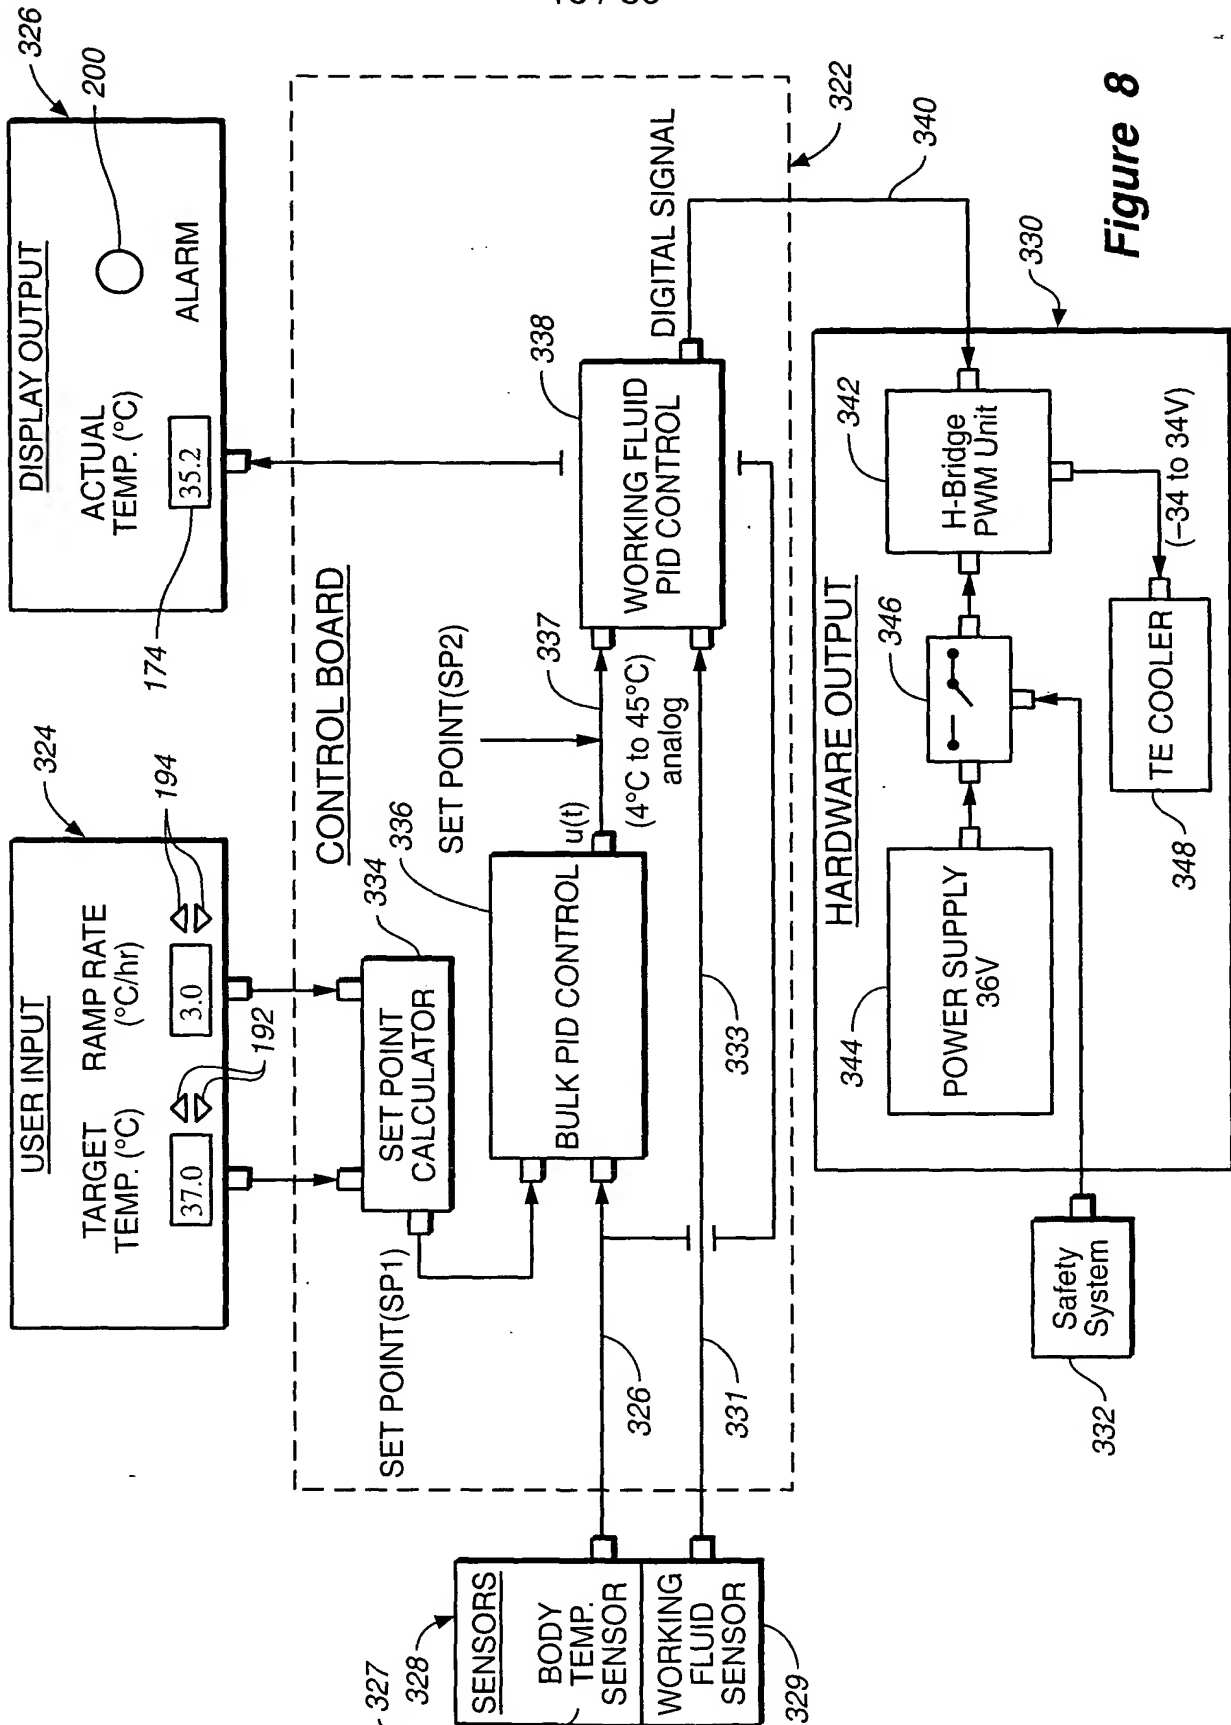


Figure 8

17 / 36



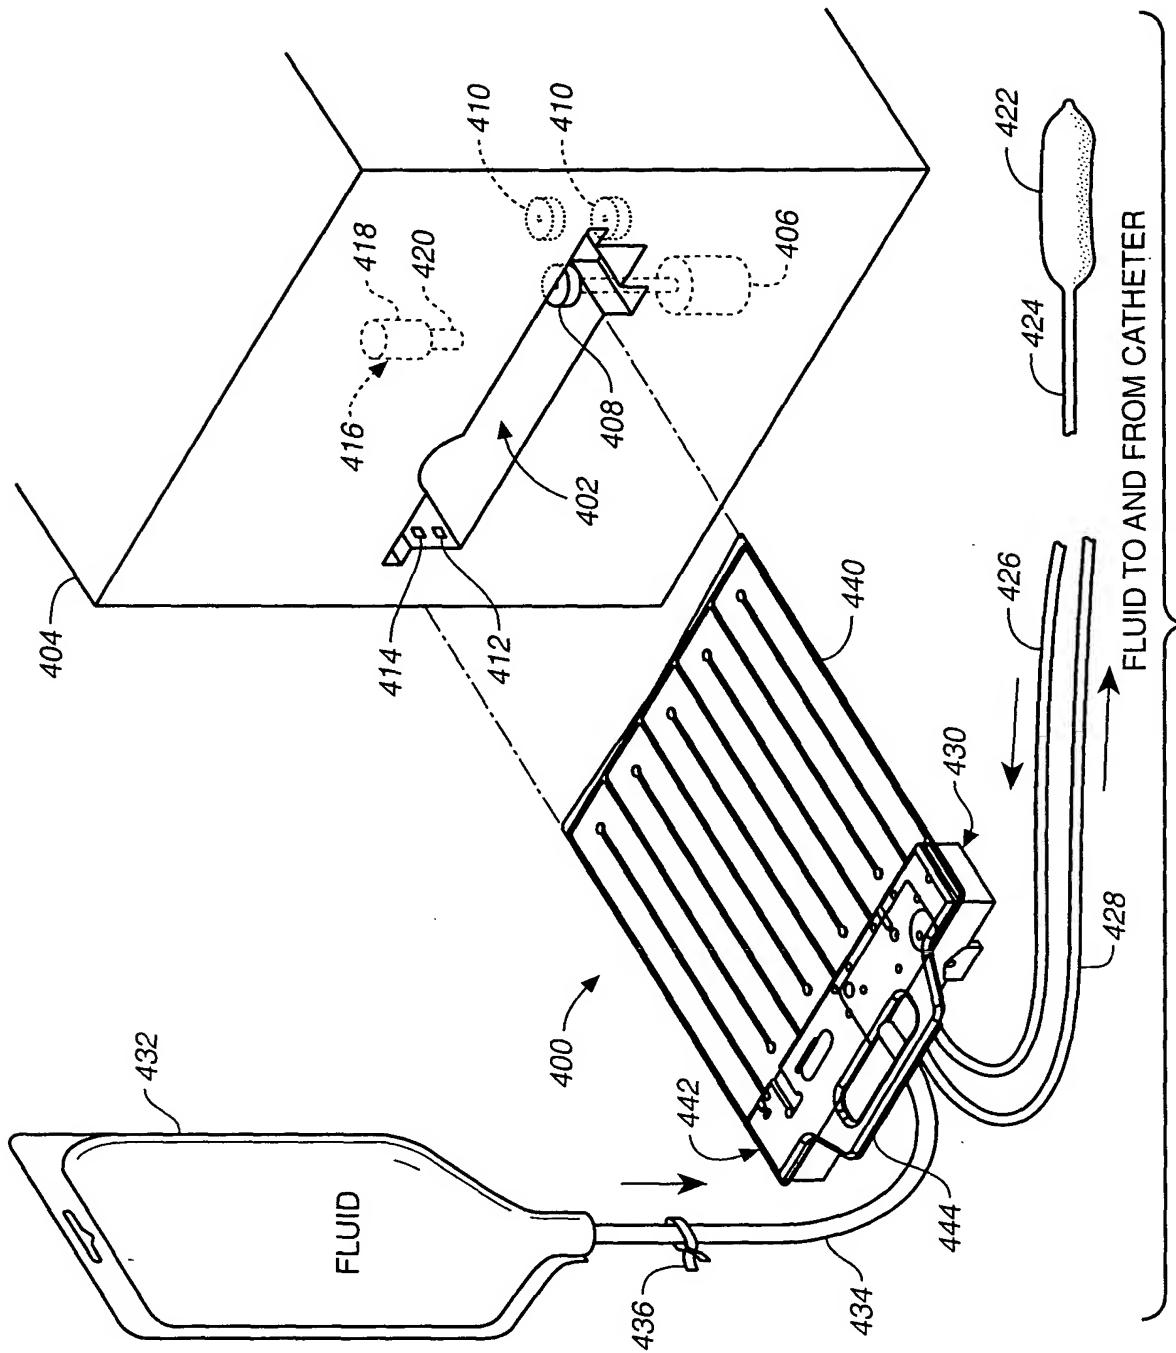


Figure 9

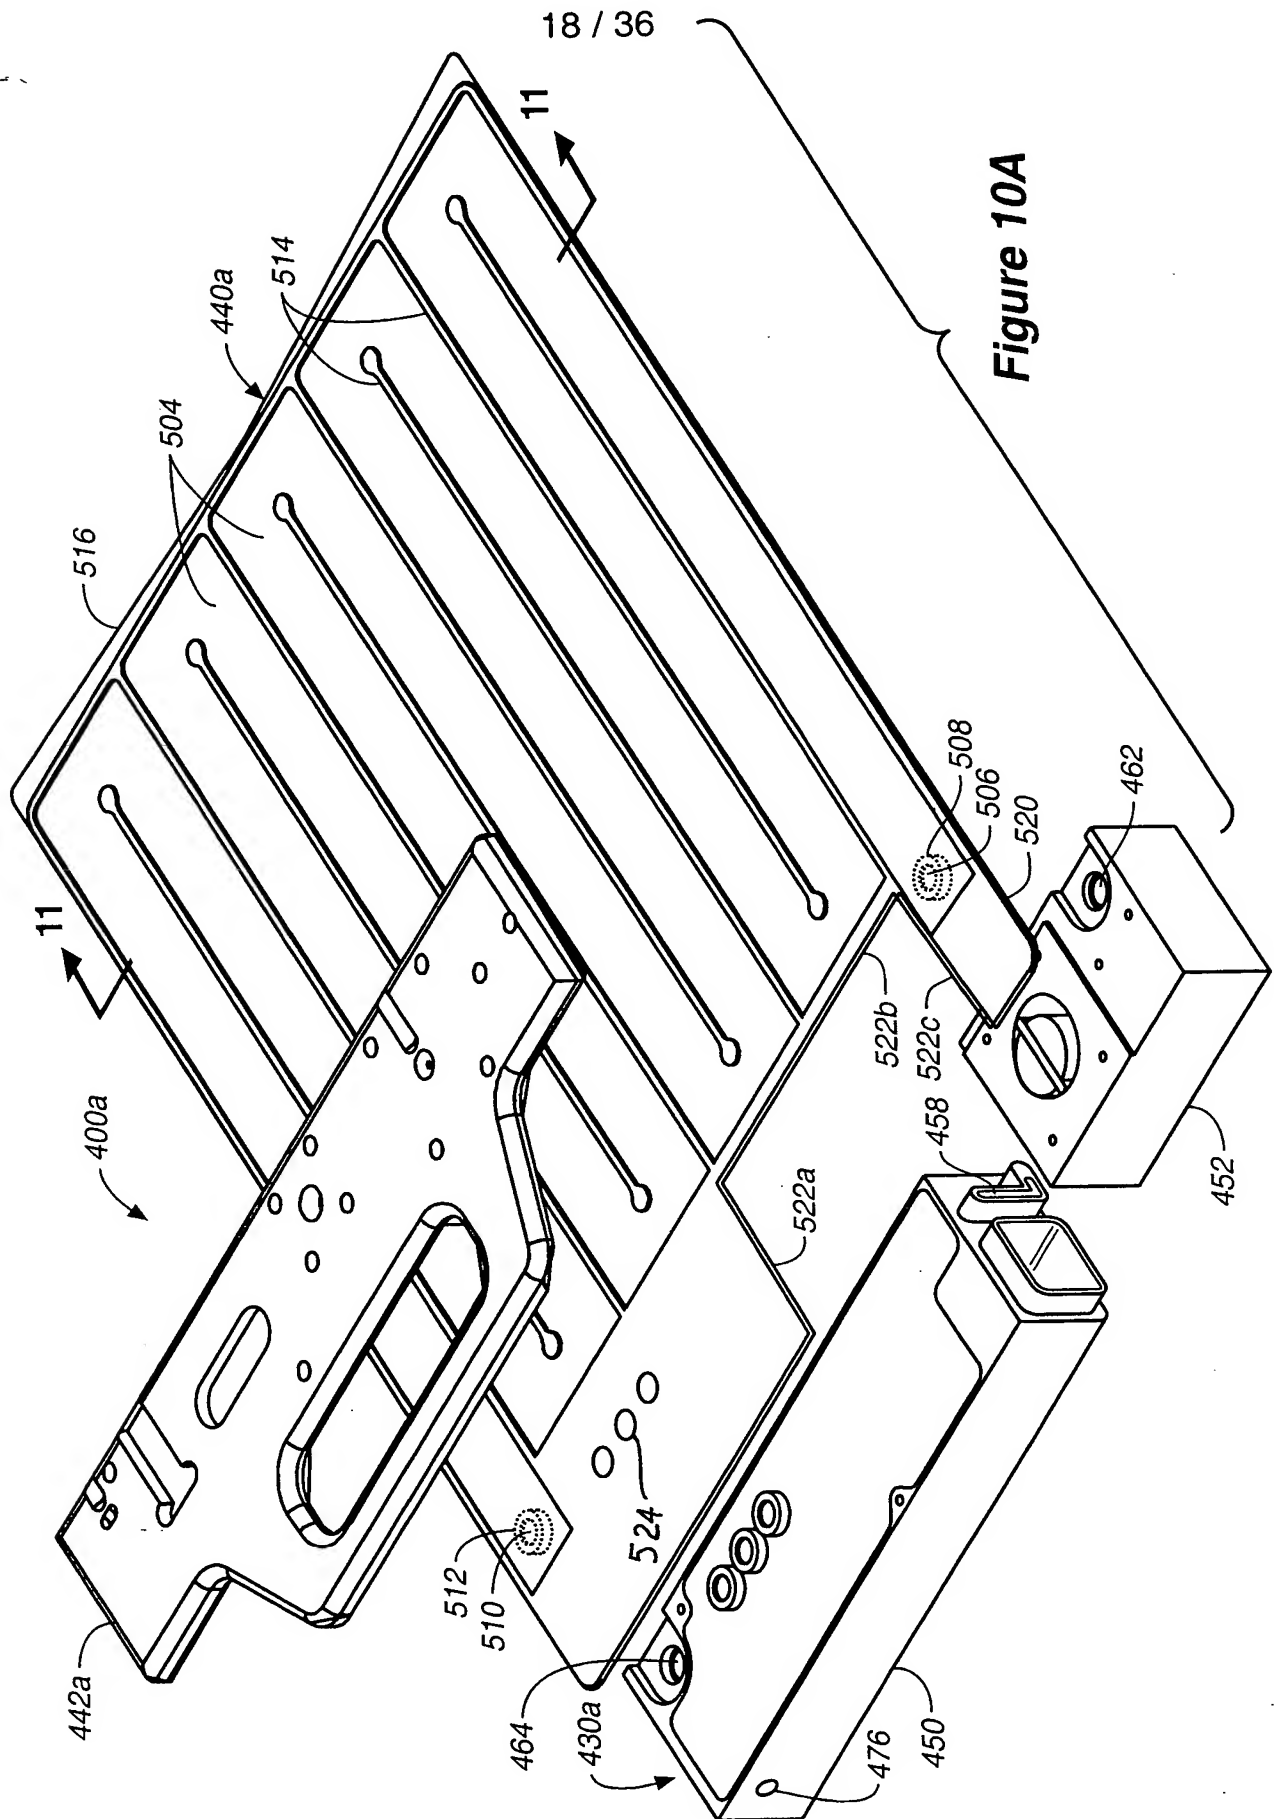

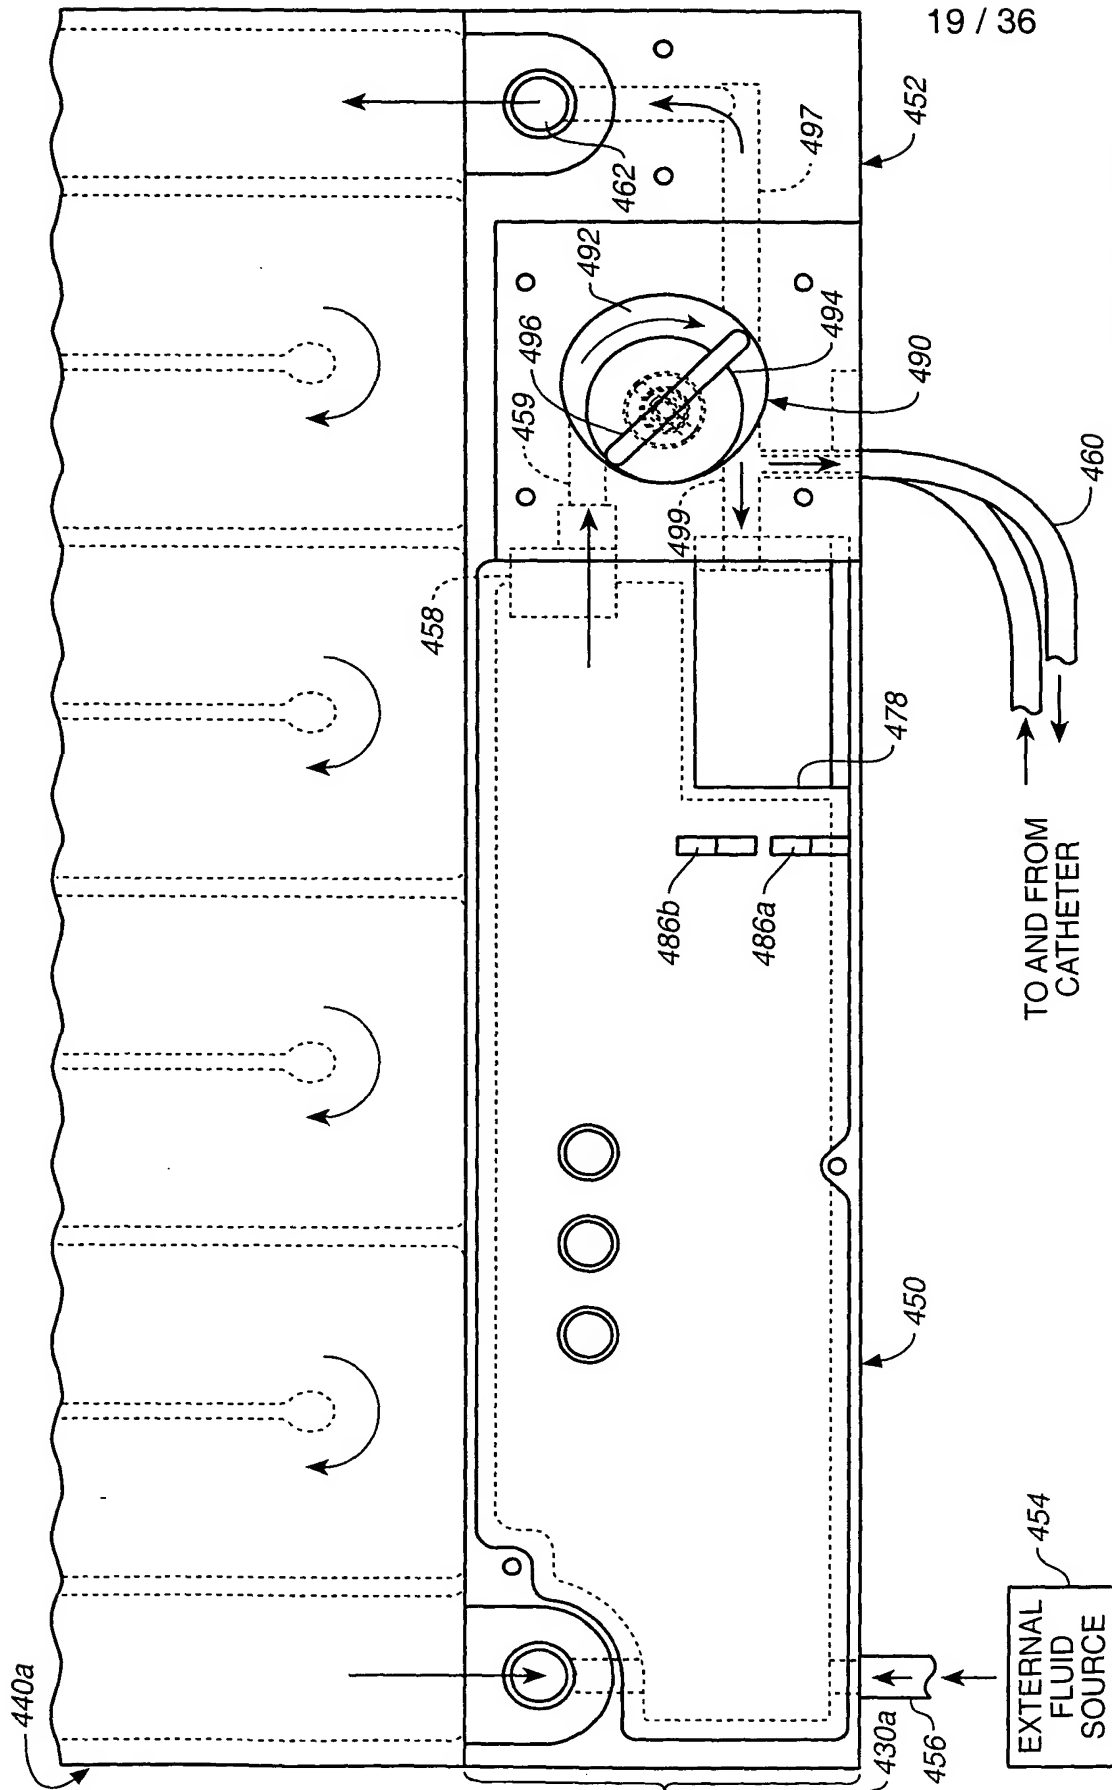

20 / 36

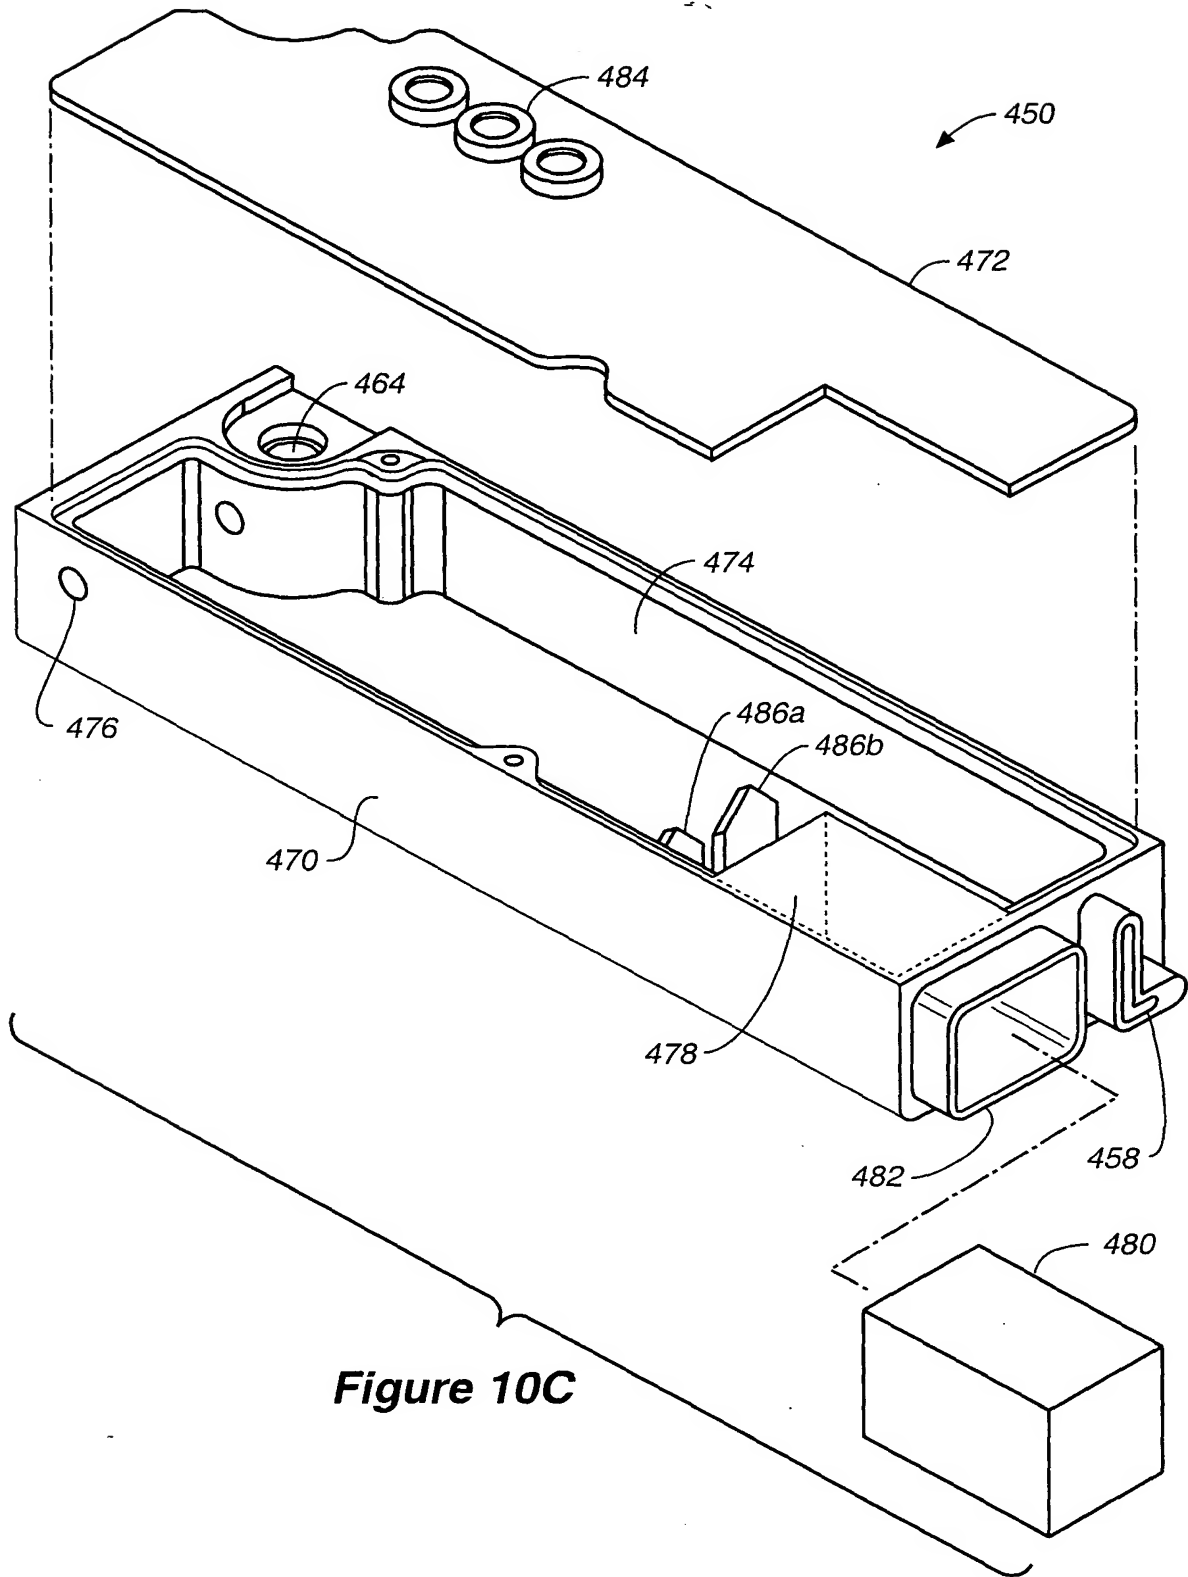
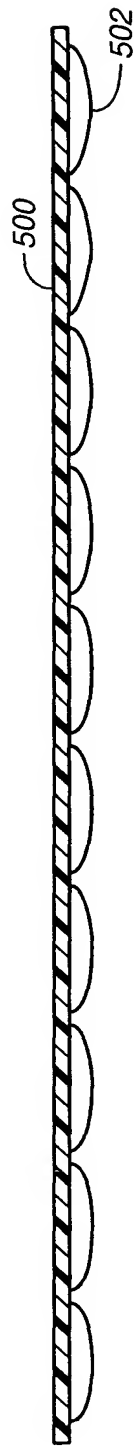
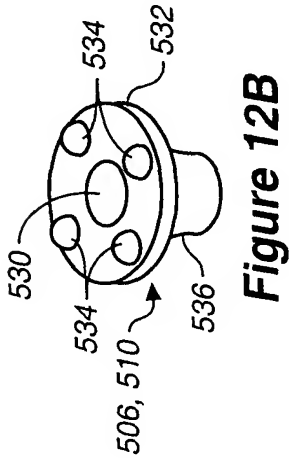
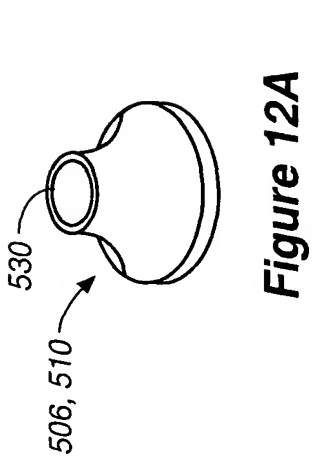
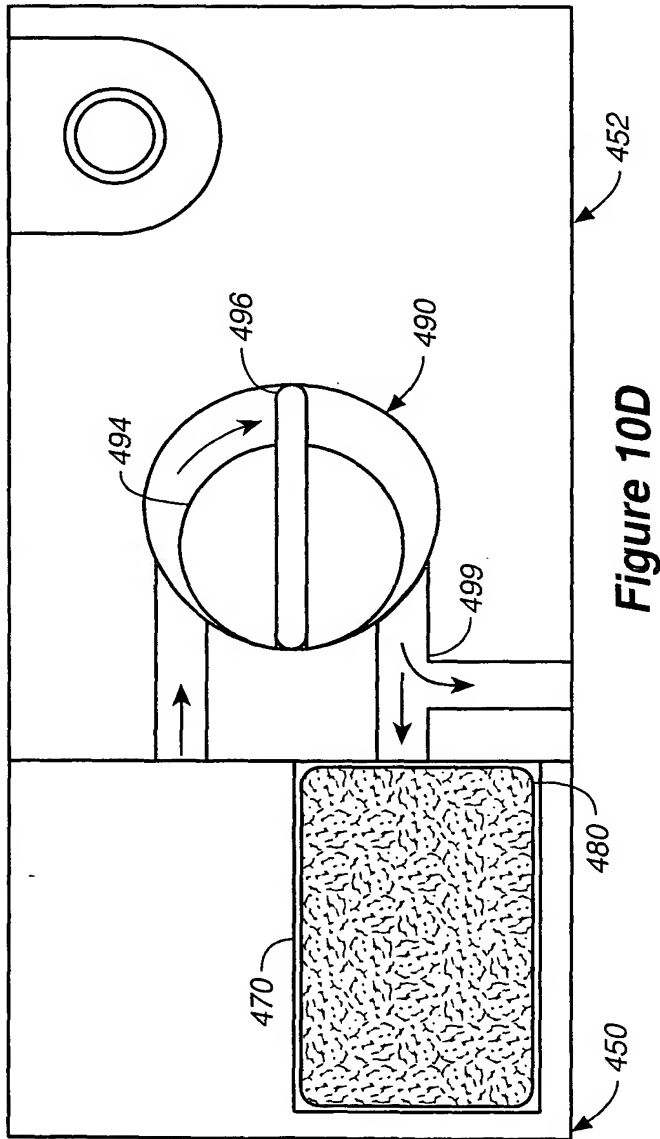


Figure 10C







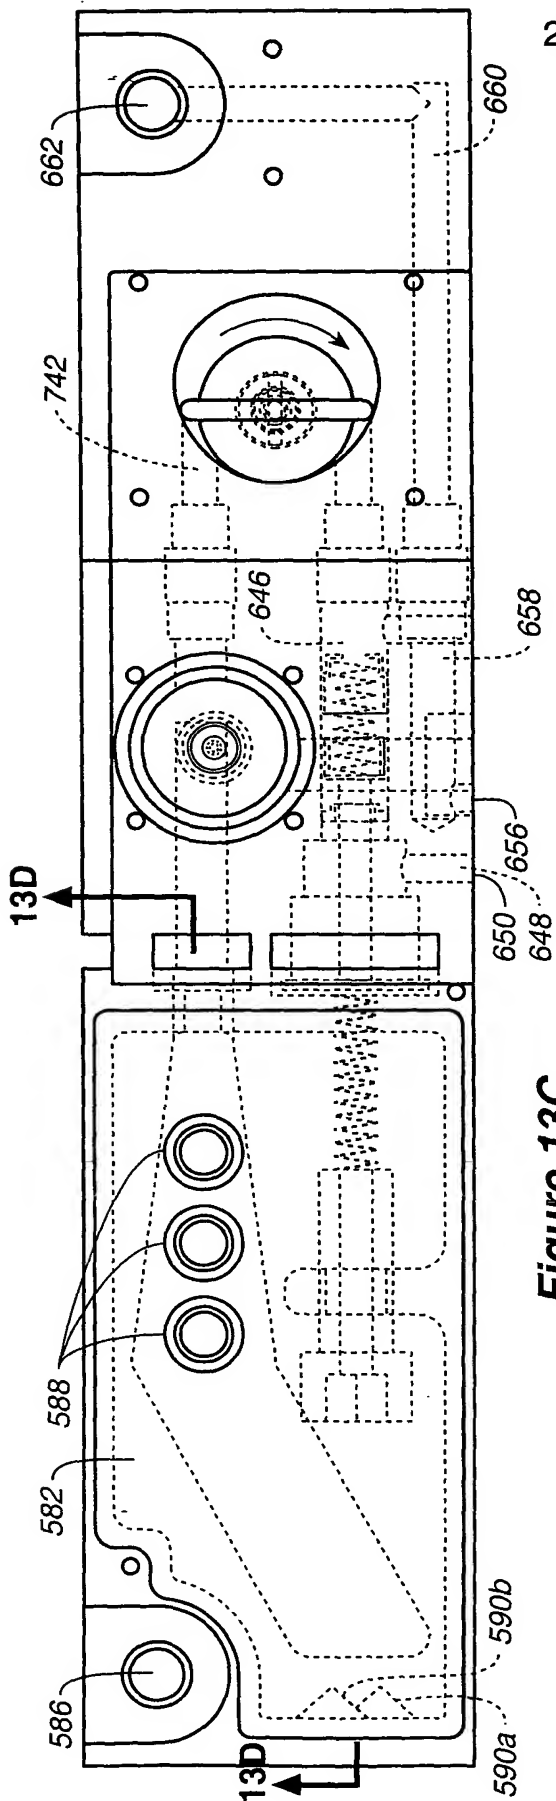


Figure 13C


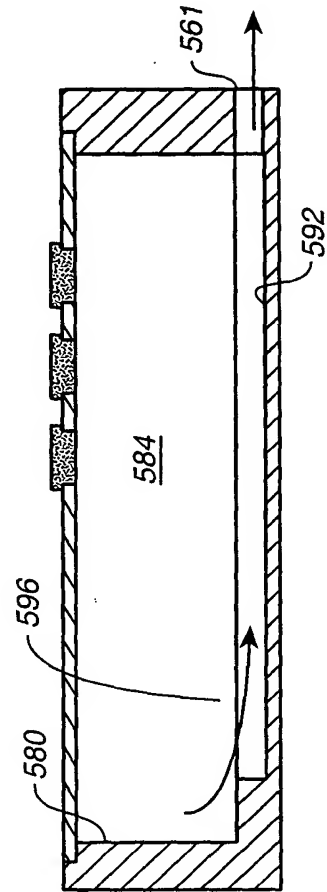


Figure 13D



Figure 13E

26 / 36

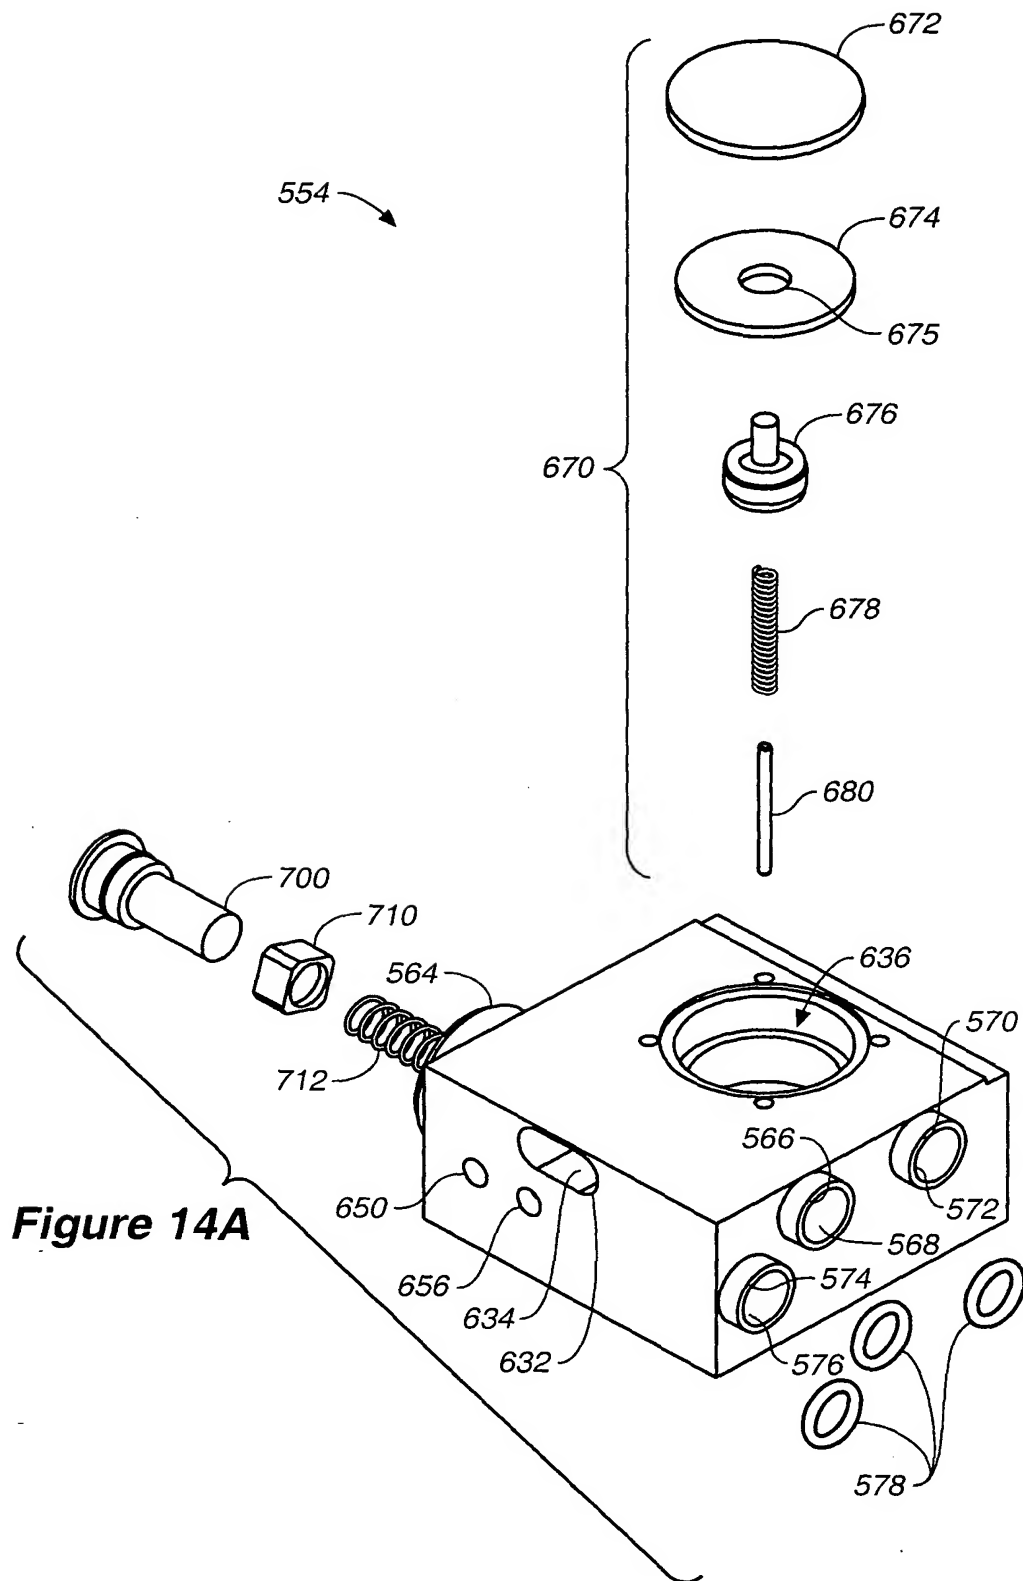

+

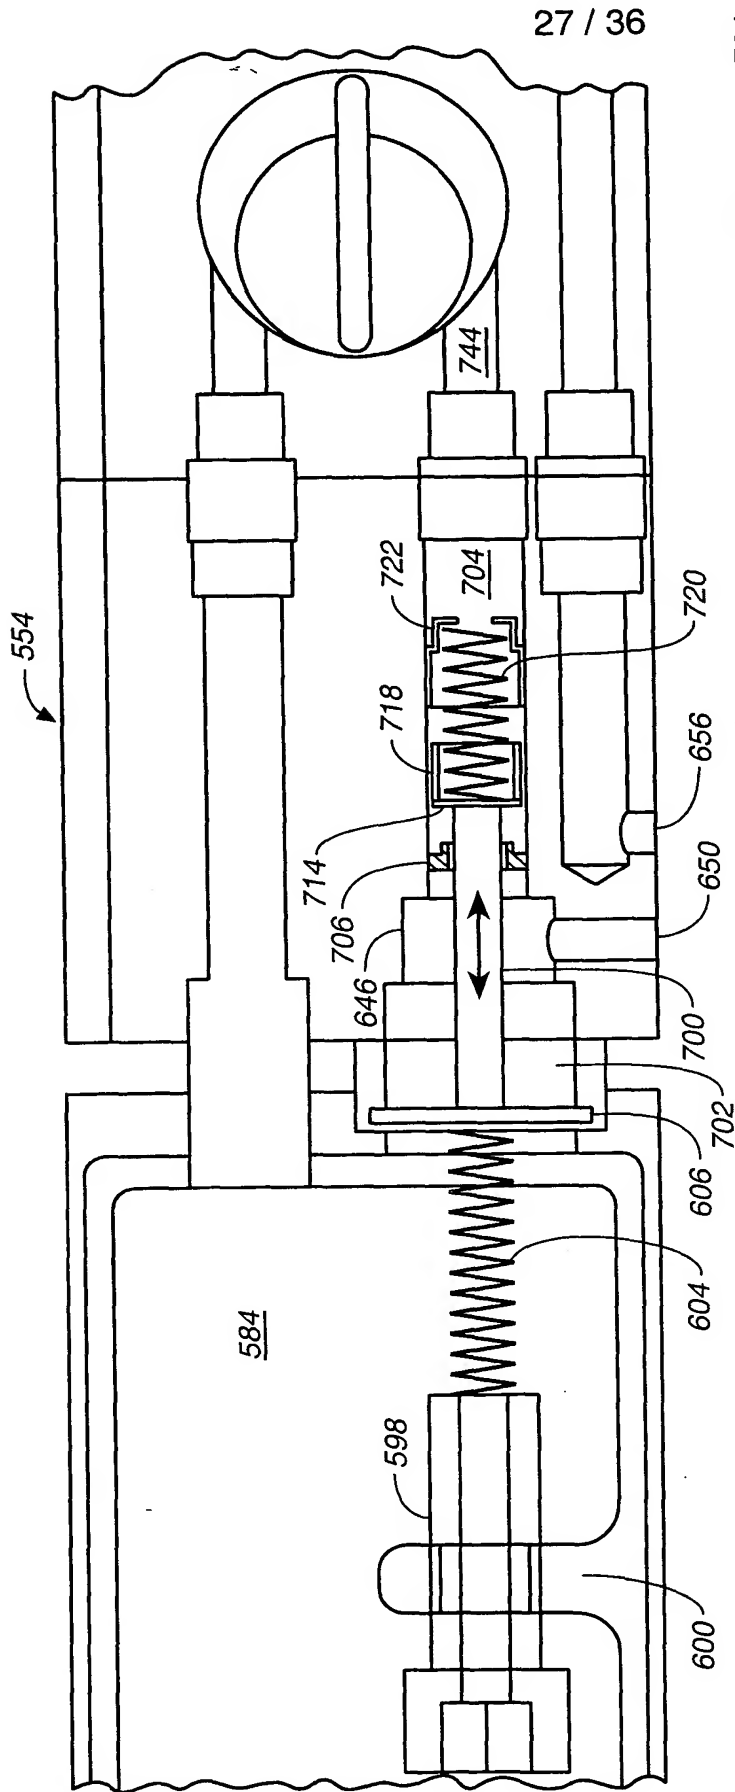


Figure 14B

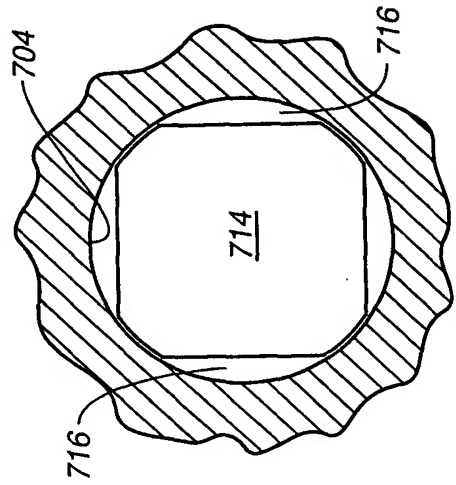


Figure 14G

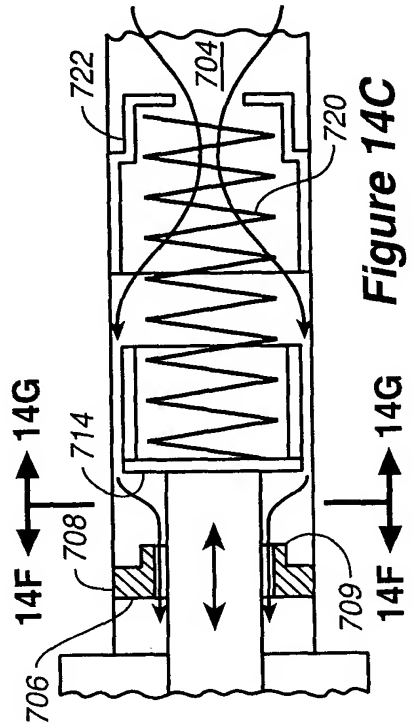


Figure 14C

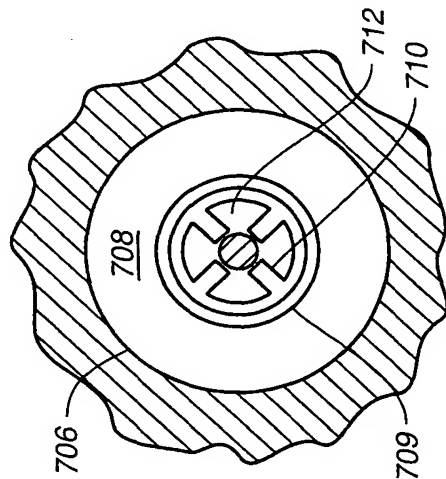


Figure 14F

+



29 / 36

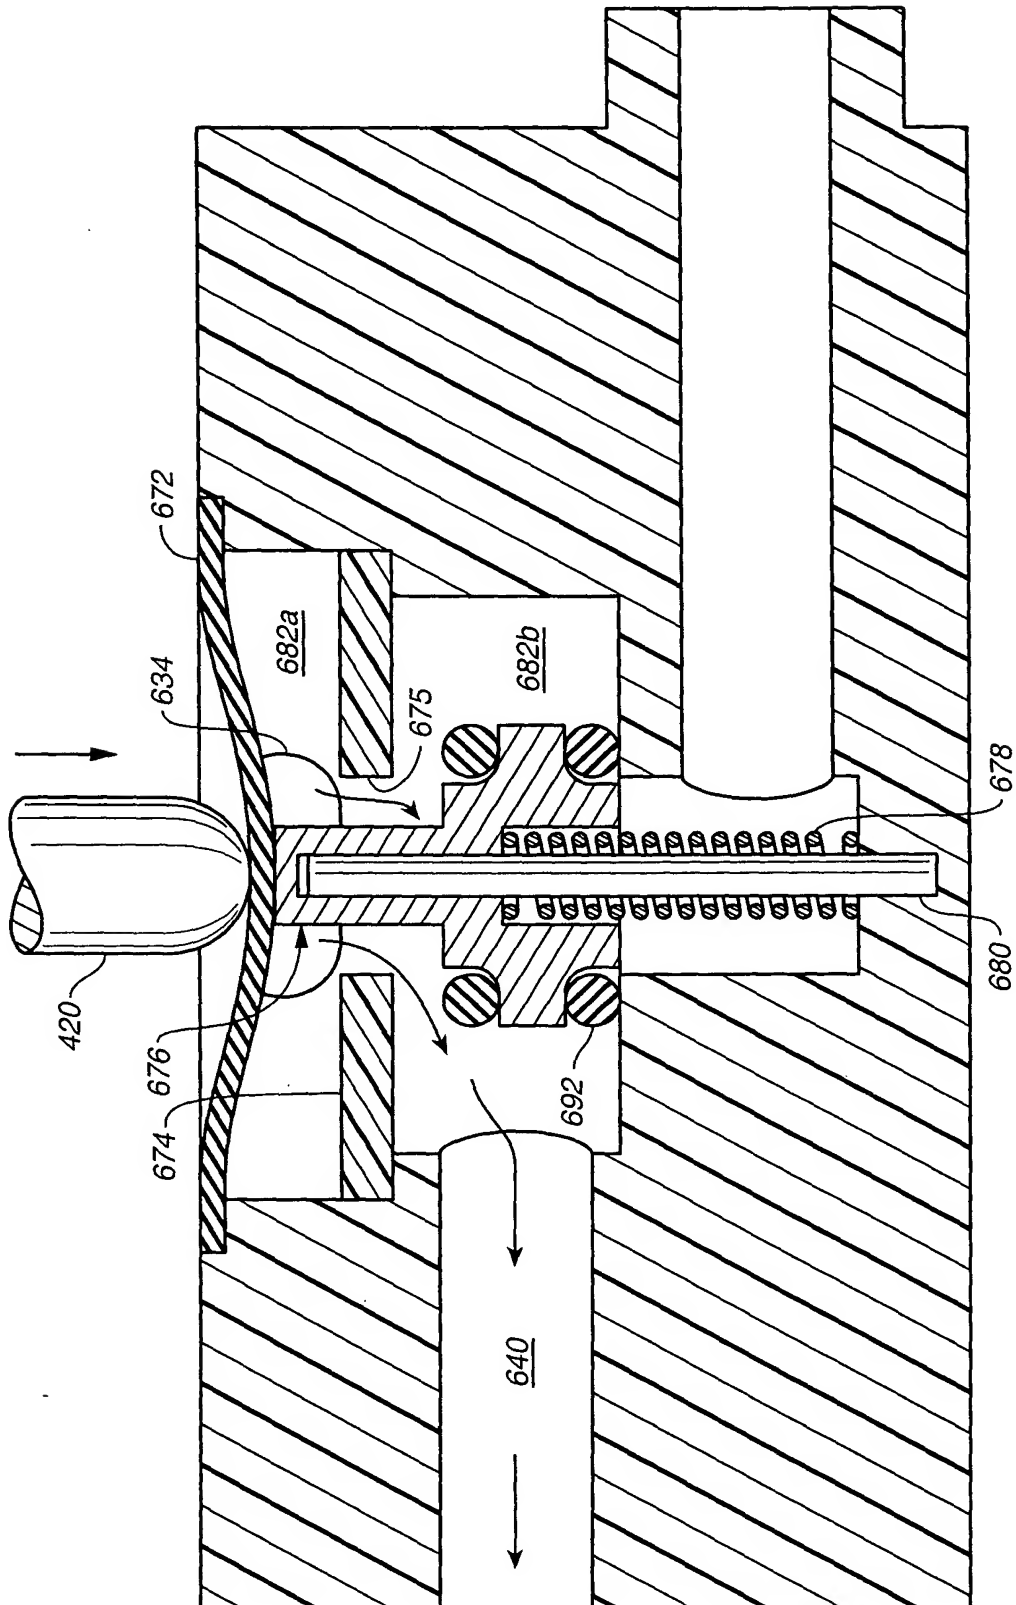


Figure 14E

30 / 36

Figure 15A

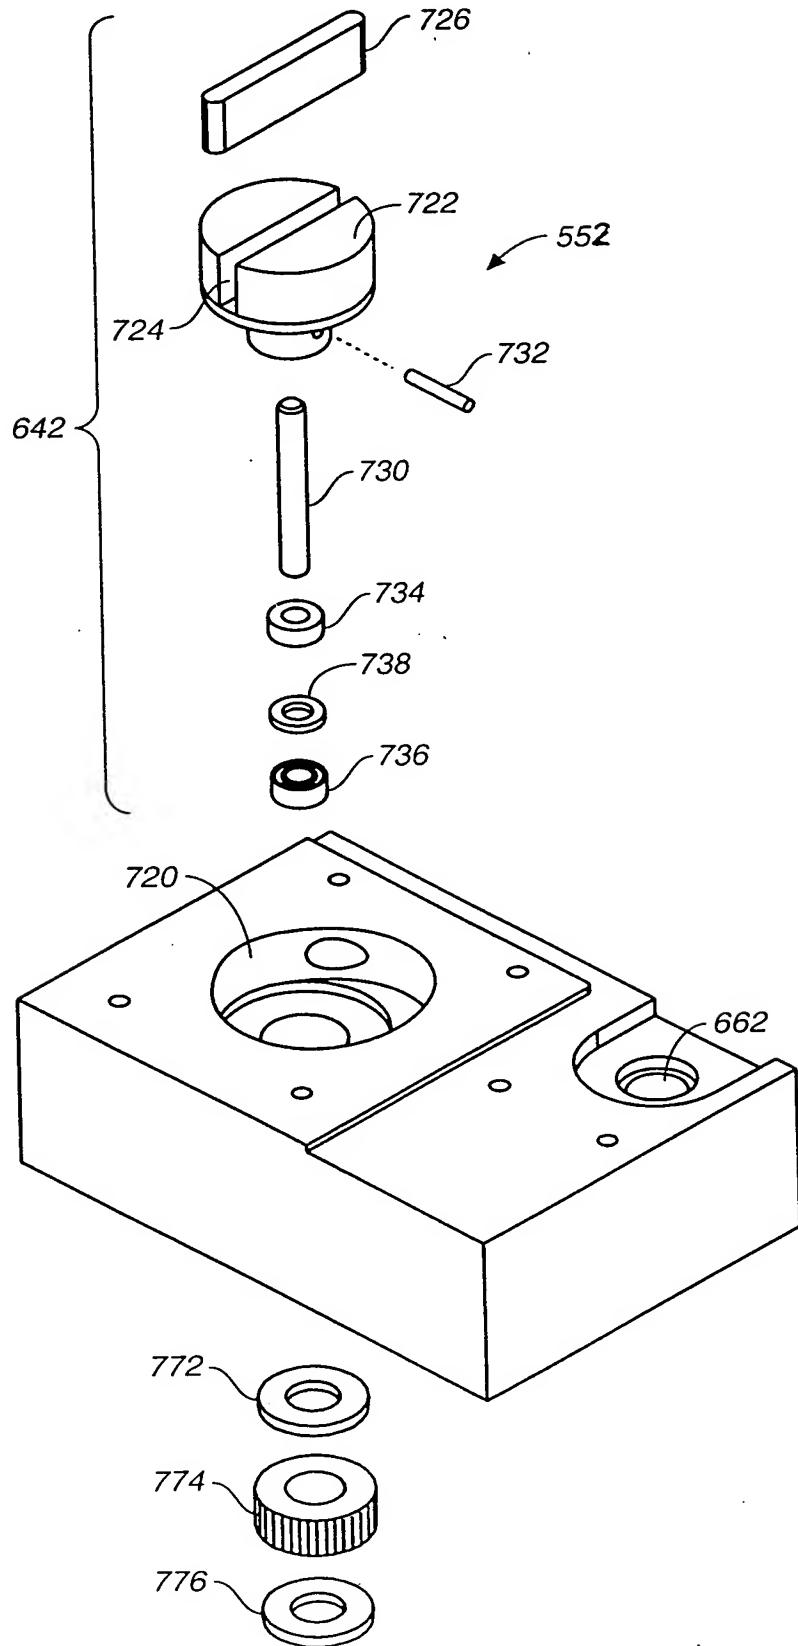








Figure 15D

34 / 36

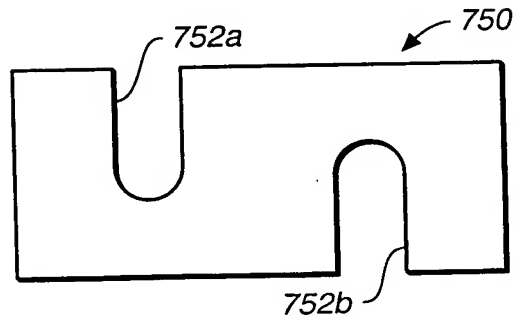


Figure 16A

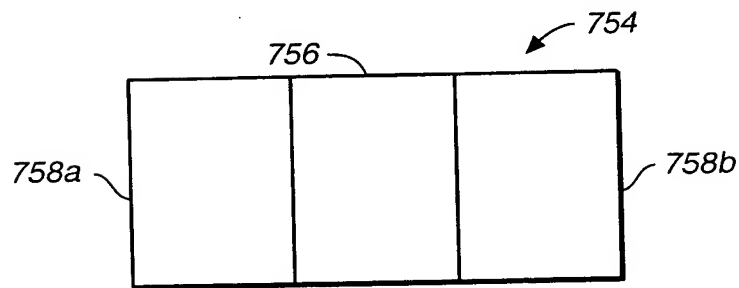


Figure 16B

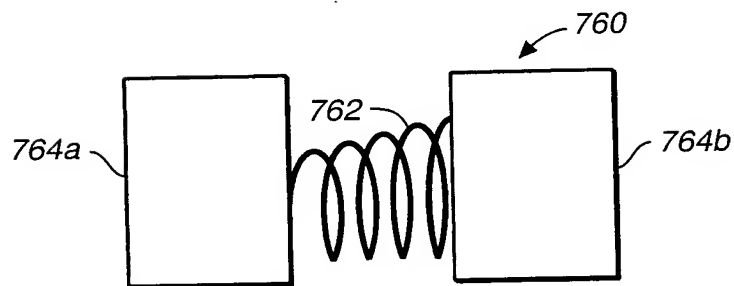


Figure 16C

35 / 36

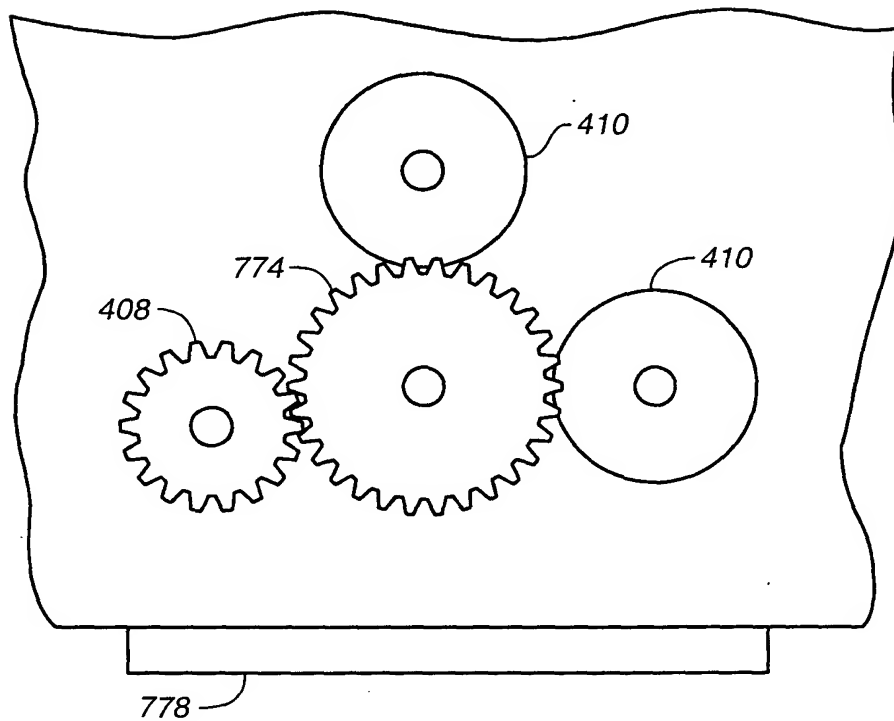


Figure 17A

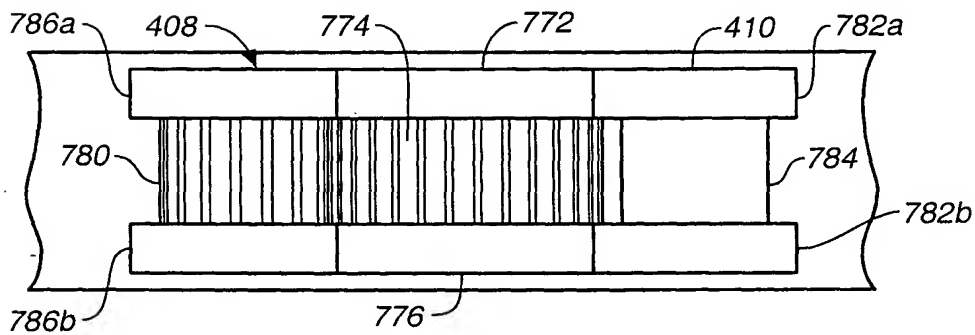


Figure 17B

36 / 36

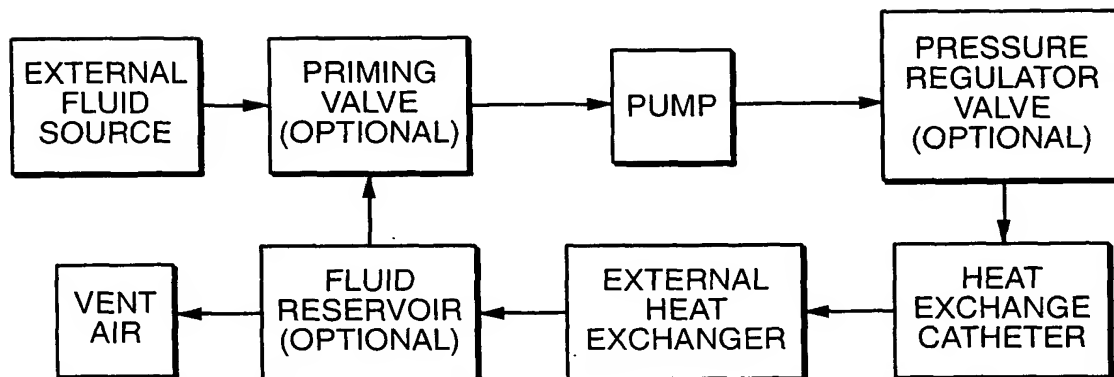


Figure 18A

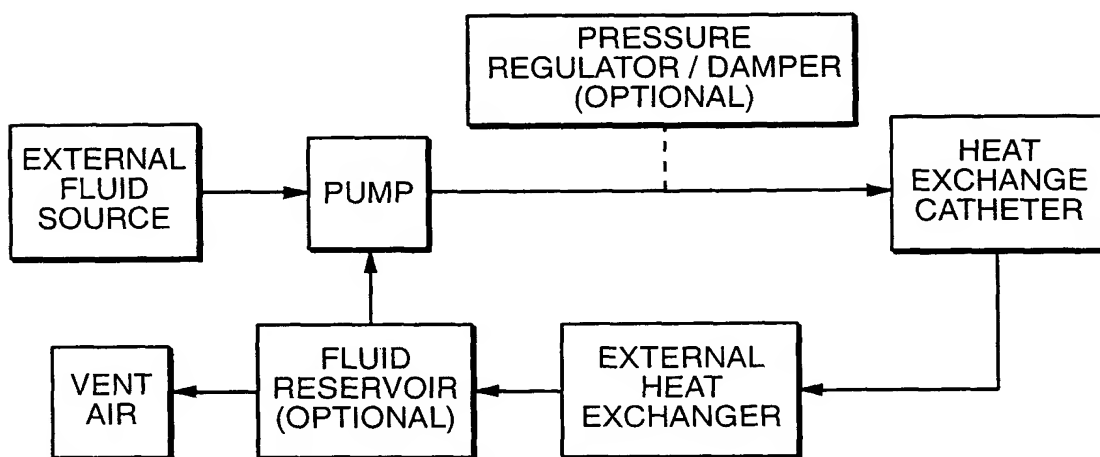


Figure 18B

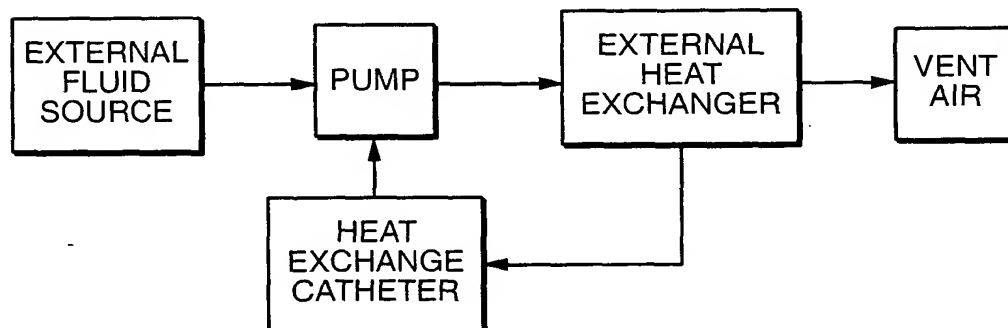


Figure 18C